

**Want More?
Solutions Start
Here!**



Introducing **BIOMET 3i**'s Product Catalog For Restorative Technologies

The Solution Designed To Provide Clinicians With Restorative Options:

- Product Innovations And Services You Can Trust
- Restorative Products That Provide End-To-End Prosthetic Solutions
- Business Excellence Solutions To Help Grow Your Practice



Providing Solutions – One **Patient** At A Time™

- Product Innovations And System Distinctions For Multiple Treatment Options
- Restorative Products Flowchart For Screw And Cement-Retained Restorations
- Restorative Products For Certain® Internal And External Hex Connection Implant Systems

BIOMET 3i™
PROVIDING SOLUTIONS – ONE PATIENT AT A TIME™

Instructions For Use

OSSEOTITE®, OSSEOTITE XP®, Certain®, PREVAIL®, Encode®, IOL®, GingiHue®, Gold-Tite®, Provide®, ZiReal®, CAM StructSURE®, NanoTite™, PreFormance®, QuickBridge®, Low Profile, Prep-Tite®, Patient Specific Restorations®, UCLA, Conical, Standard, LOCATOR®, OverdentSURE

This document applies to dental implants, abutments, overdenture bars and associated surgical, restorative and dental laboratory components.

For detailed information on the specific procedure for the product you are using, please refer to the individual product labels and/or the appropriate manual.

Description: BIOMET **3i** Dental Implants are manufactured from biocompatible titanium or titanium alloy and abutments from titanium, titanium alloy, gold alloy and ceramic material. BIOMET **3i** Dental Implants and Abutments include various surface treatments and coatings. Other restorative components are manufactured from titanium, titanium alloy, gold alloy, stainless steel and a variety of polymers.

For specific product description and net quantity, refer to individual product labels.

Indications for Use: BIOMET **3i** Dental Implants are intended for surgical placement in the upper or lower jaw to provide a means for prosthetic attachment in single tooth restorations and in partially or fully edentulous spans with multiple single teeth utilizing delayed or immediate loading, or with a terminal or intermediary abutment for fixed or removable bridgework, and to retain overdentures.

BIOMET **3i** OSSEOTITE® and NanoTite™ Dental Implants are intended for immediate function on single tooth and/or multiple tooth applications when good primary stability is achieved, with appropriate occlusal loading, in order to restore chewing function.

Additional Indications: BIOMET **3i** Dental Abutments and Overdenture Bars are intended for use as an accessory to endosseous dental implants to support a prosthetic device in a partially or edentulous patient. These are intended for use to support single and multiple tooth prostheses, in the mandible or maxilla. The prostheses can be screw or cement retained to the abutment.

PEEK Abutment Posts and Temporary Cylinders are intended for use as an accessory to endosseous dental implants to support a prosthetic device in a partially or fully edentulous patient. These are intended for use to support single and multiple unit prostheses in the mandible or maxilla for up to 180 days during endosseous and gingival healing, and are for non occlusal loading of single and multiple unit provisional restorations. The prostheses can be screw and/or cement retained to the abutment. These Temporary Posts and Cylinders require a minimum interarch space of 6mm and a maximum angulation of 15°. These also allow for occlusal loading of single and multiple unit restorations of integrated implants for guided soft tissue healing.

The QuickBridge® Provisional Components are intended to be mated with BIOMET **3i** Conical Abutments for use as an accessory to endosseous dental implants to support a prosthetic device in a partially or fully edentulous patient. The QuickBridge® Provisional Components are intended to support multiple unit prostheses in the mandible or maxilla for up to 180 days during endosseous and gingival healing.

BIOMET **3i** Low Profile Abutments are intended for use as accessories to endosseous dental implants to support a prosthetic device in a partially or completely edentulous patient. A dental abutment is intended for use to support single and multiple tooth prostheses, in the mandible or maxilla. The prosthesis can be screw or cement retained to the abutment.

Contraindications: Placement of dental implants may be precluded by patient conditions that are contraindications for surgery. BIOMET **3i** Dental Implants should not be placed in patients where the remaining jaw bone is too diminished to provide adequate implant stability.

Storage and Handling: Devices should be stored at room temperature. Refer to individual product labels and the Surgical Manual for special storage or handling conditions.

Warnings: Excessive bone loss or breakage of a dental implant or restorative device may occur when an implant or abutment is loaded beyond its functional capability. Physiological and anatomic conditions may negatively affect the performance of dental implants. The following should be taken into consideration when placing dental implants:

- Bone quality
- Oral hygiene
- Medical conditions such as blood disorders or uncontrolled hormonal conditions

It is recommended that small diameter implants not be restored with angled abutments in the molar region.

Mishandling of small components inside the patient's mouth carries a risk of aspiration and/or swallowing.

Forcing the implant into the osteotomy deeper than the depth established by the drills can result in: stripping the driver hex interface inside the implant, stripping the driver, coldwelding of the mount-driver interface to the implant, or stripping the walls of the osteotomy that may prevent an effective initial implant fixation.

Precautions: For safe and effective use of BIOMET **3i** Dental Implants, abutments and other surgical and restorative dental accessories, these products or devices should only be used by trained professionals. The surgical and restorative techniques required to properly utilize these devices are highly specialized and complex procedures. Improper technique can lead to implant failure, loss of supporting bone, restoration fracture, screw loosening and aspiration.

Reuse of BIOMET 3i products that are labeled for single-use may result in product contamination, patient infection and/or failure of the device to perform as intended.

Sterility: All dental implants and some abutments are supplied sterile and are sterilized by an appropriate validated method. Refer to individual product labels for sterilization information; all sterile products are labeled 'STERILE.' All products sold sterile are for single use before the expiration date printed on the product label. Do not use sterile products if the packaging has been damaged or previously opened. Do not re-sterilize or autoclave except where instructions to do so are provided on the product label, in the Surgical Manual, in the Restorative Manual or in any additional marketing literature for that product. Products provided non-sterile must be cleaned and sterilized according to the directions found in ART630 or the Surgical Manual prior to use.

Procedural Precautions, Surgery: For a detailed explanation of the procedural precautions refer to the Surgical Manual. During the planning phase, it is important to determine the vertical dimension, the actual space available between the alveolar crest and the opposing dentition, in order to confirm that the available space will accommodate the proposed abutment and the final crown restoration. This information varies with each patient and abutment; therefore it should be carefully evaluated before placing any dental implant. Utilize continuous irrigation with a cool, sterile irrigating solution to avoid excessive damage to the surrounding tissue and to prevent compromising osseointegration. This is mandatory during all procedures. Avoid excessive pressure during preparation of the bone site. As the drilling speed varies based on the instrument and the surgical procedure, recommendations for speed can be found in the Surgical Manual. Only sharp instruments of the highest quality should be used for any surgical procedure involving bone. Minimizing trauma to the bone and surrounding tissue enhances the potential for successful osseointegration. In order to eliminate contaminants and other sources of infection, all non-sterile devices should be cleaned and/or sterilized prior to use, per the instructions on the individual product labels.

Procedural Precautions, Restoration: The healing period varies depending on the quality of the bone at the implantation site, the tissue response to the implanted device and the surgeon's evaluation of the patient's bone density at the time of the surgical procedure. Excessive force applied to the dental implant should be avoided during the healing period. Proper occlusion should be evaluated on the implant restoration to avoid excessive force.

Potential Adverse Events: Potential adverse events associated with the use of dental implants may include:

- Failure to integrate
- Loss of integration
- Dehiscence requiring bone grafting
- Perforation of the maxillary sinus, inferior border, lingual plate, labial plate, inferior alveolar canal, gingiva
- Infection as reported by: abscess, fistula, suppuration, inflammation, radiolucency
- Persistent pain, numbness, paresthesia
- Hyperplasia
- Excessive bone loss requiring intervention
- Implant breakage or fracture
- Systemic infection
- Nerve injury

Caution: U.S. Federal Law restricts this device to sale by or on the order of a licensed dentist or physician.

Table Of Contents

Introduction

Company Overview	i
Product Innovations Timeline	ii
System Distinctions	iii
Patient Specific Restorations® Overview	v

Restorative Products Flowchart

Cement-Retained Restoration Details	1
Screw-Retained Restoration Details	1
Provide® Abutment Selection Guide	2

Restorative Products

Certain® Internal Connection:

Cement-Retained Restorations	
Provide Abutments	3
GingiHue® Posts	5
ZiReal® Posts	7
UCLA Abutments	9

Screw-Retained Restorations	
UCLA Abutments	11
Low Profile Abutments	13
Immediate Occlusal Loading (IOL®) Abutments	15
Conical Abutments	17

OverdentSURE Restorations	
DIEM® IOL Abutments	19
Standard Abutments	21
LOCATOR® Abutments	23

Provisional Restorations	
PreFormance® Posts	25
PreFormance Temporary Cylinders	26

External Hex Connection:

Cement-Retained Restorations	
GingiHue Posts	27
ZiReal Posts	29
UCLA Abutments	31

Screw-Retained Restorations	
UCLA Abutments	33
Low Profile Abutments	35
Immediate Occlusal Loading (IOL) Abutments	37
Conical Abutments	39

OverdentSURE Restorations	
DIEM Immediate Occlusal Loading (IOL) Abutments	41
Standard Abutments	43
LOCATOR Abutments	45
O-Ring Abutments	47
Dal-Ro Abutments	49

Provisional Restorations	
PreFormance Posts	51
PreFormance Temporary Cylinders	52

Miscellaneous Restorative Products	
Screws	53
Mechanical Driver Kits	55
Drivers And Driver Tips	56
Navigator® System Instrumentation Overview	57
Navigator Laboratory Kit	58
Laboratory Tools/Miscellaneous Items	59

Professional Development Products	
Tools For The Art Of Business Building	60

Additional Information	
Index	61
Ordering Form	
Ordering Information	

Introduction

Company Overview

BIOMET 3i™ Providing Solutions – One Patient At A Time™

Mission Statement:

BIOMET 3i will be recognized as a global leader in the oral reconstruction marketplace. We will achieve this through superior customer support and continuous product innovation.

BIOMET 3i offers one of implant dentistry's most comprehensive lines of implants and abutments, augmented by a growing line of site preparation and regenerative products. BIOMET 3i pioneered the development of biologically driven implants, winning worldwide acclaim for the microtextured surface and superior clinical success rates of the OSSEOTITE® Implant.

Headquartered in Palm Beach Gardens, Florida, with operations throughout the world, BIOMET 3i is one of the leading companies in the oral reconstruction market. Of equal importance, BIOMET 3i brings the same innovation, high standards and comprehensive approach to customer service, practice and laboratory support and education.

Our Solutions Offer:

Comprehensive Treatment


- Patient Driven Implant Systems
- End-To-End Prosthetic Solutions
- Site-Specific Regenerative Options

Enhanced Knowledge

- Comprehensive Educational Continuum For All Levels Of Expertise
- Diversified Delivery Options
- Audience-Specific Program Options

Business Excellence

- Patient Recruitment Support
- Business Efficiency Support
- Practice Growth Support

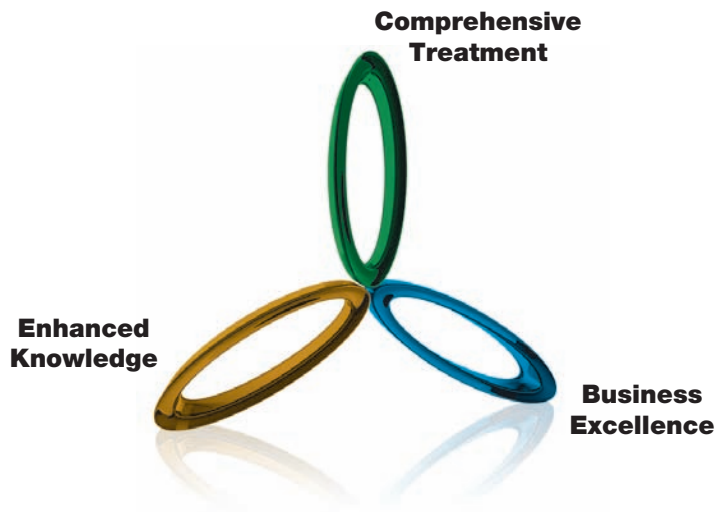

Introduction



Product Innovations Timeline - 1987 To Present

1987	1988	1989	1990
<ul style="list-style-type: none"> • 2mm Standard Abutments • One-Piece Abutment Posts 	<ul style="list-style-type: none"> • Machined Gold UCLA Abutments • Modification Abutments • 2.9mm Miniplants® • Pre-Angled Abutments 	<ul style="list-style-type: none"> • Tapered Abutments • 3.75mm Threaded Implants 	<ul style="list-style-type: none"> • EP® Healing Abutments
1991	1992	1993	1994
<ul style="list-style-type: none"> • Wide Diameter Implants 	<ul style="list-style-type: none"> • Conical Abutments For Single-Unit Applications 	<ul style="list-style-type: none"> • Protocol For Single-Stage Surgery With Hex Top Implants • Two-Piece EP Healing Abutments • Two-Piece Abutment Posts 	<ul style="list-style-type: none"> • Emergence Profile System • EP Abutment Posts • STA Abutments
1995	1996	1997	1998
<ul style="list-style-type: none"> • ASYST Abutment Delivery System • Twist Lock™ Impression Copings • ICET™ Implants 	<ul style="list-style-type: none"> • OSSEOTITE® Implants • Gold Standard ZR™ Hex Machining 	<ul style="list-style-type: none"> • TG OSSEOTITE® Single-Stage Implants 	<ul style="list-style-type: none"> • Prep-Tite® Posts • Gold-Tite® Screws • Biogran® Bone Graft Material
1999	2000	2002	2003
<ul style="list-style-type: none"> • GingiHue® Posts • 15° Pre-Angled GingiHue Posts • Prep-Tite Caps • Try-In Screw With One Turn • OSSEOTITE XP® Implants • Restorative Torque Indicator 	<ul style="list-style-type: none"> • ZiReal® Posts • Simple Logic™ • PCCS® Platelet Concentrate Collection System 	<ul style="list-style-type: none"> • LOCATOR® Abutments • Safescraper® Bone Collector • Tapered Implant System • Calcigen™ Oral Bone Graft Stabilizer 	<ul style="list-style-type: none"> • OSSEOTITE Certain® Internal Connection Implant System With The QuickSeat® Connection • OverdentSURE Approach
2004	2005	2006	2007
<ul style="list-style-type: none"> • DIEM® Immediate Occlusal Loading Guidelines & IOL® Components • ARCHITECH PSR®: CAM StructSURE® Precision Milled Bars, Encode® Restorative System 	<ul style="list-style-type: none"> • 3i IDS Learning Library® • PREVAIL® Implants • Provide® Abutments 	<ul style="list-style-type: none"> • Advanced Cutting Technology® (ACT™) Twist Drills • OSSEOCISION® Drilling Unit • PreFormance® Provisional Components 	<ul style="list-style-type: none"> • NanoTite™ Implants • Conical Angled Abutments • QuickBridge® Provisional Components • OsseoGuard® Membrane
2008	2009	2010	
<ul style="list-style-type: none"> • Navigator® System For Guided Surgery • NanoTite Tapered PREVAIL Implants • Encode Complete • RegenerOss® Family Of Products 	<ul style="list-style-type: none"> • Low Torque Indicating Ratchet Wrench 	<ul style="list-style-type: none"> • Larger Particle Size Endobon® Xenograft Granules • Low Profile Abutments 	


Introduction

System Distinctions


Certain® Internal Connection Implants

The internal connection implant design is for ease of use and simplicity.


Material: Titanium Alloy

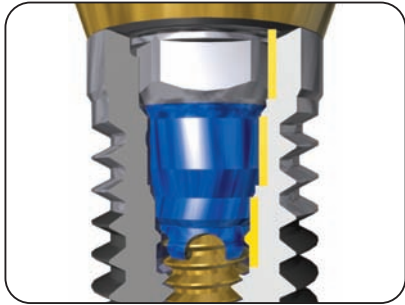

- QuickSeat® Connection: It Clicks! The Certain Implant System features the QuickSeat Connection, which has an audible and tactile “click” when placing impression copings and abutments. This click feedback provides confirmation and confidence to a clinician that the components are properly seated. *When It Clicks, It's Seated. You're Certain.*

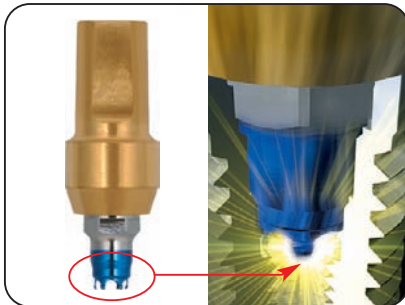

- Abutment fingers cause the “click” and also provide retention for the prosthetic components in the implant when restorations are being tried in or placed before the screw is placed.

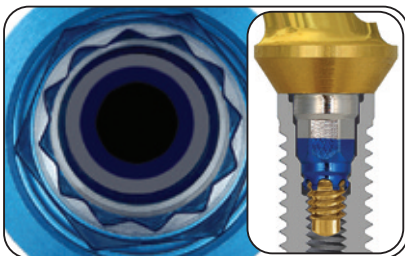

- The 6/12 internal connection has both a 6-point hex and a 12-point double hex. The 6-point hex has two functions: engaging the driver tip for mountless delivery during implant placement and providing anti-rotation for all straight abutments. The 12-point double hex provides rotational positioning every 30° for pre-angled abutments.



- Impression Copings: Pick-Up and Twist Lock™ Transfer Copings are available in the internal connection design. The impression copings also “click” when properly seated. The copings have a different finger design that engages 2mm internally in the implant, as compared to the abutment's design that engages 4mm deep in the implant. This shorter engagement in the implant is important because it allows off-axis draw for impressions of divergent implants.


Introduction

System Distinctions


External Hex Connection Implants

The external hex implant design is widely used offering versatility and restorative flexibility.

Material: Commercially Pure Titanium (OSSEOTITE® Implants)
Titanium Alloy (NanoTite™ Implants)

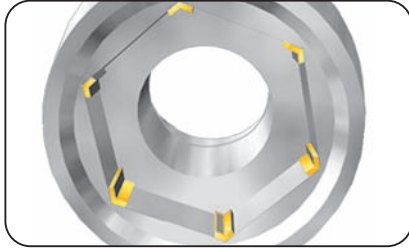

- Gold Standard ZR™ (Zero Rotation) is a patented design of machined microstops within the corners of the hex in the abutment. The design reduces horizontal rotation between the implant and abutment. Gold Standard ZR is available on UCLA, GingiHue® Post and Conical Abutments.

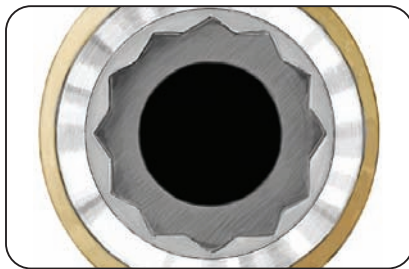

- The 12-point double hex, which is machined in the 15° Pre-Angled GingiHue Post, provides rotational positioning in 30° increments on the implant hex.



- Impression Copings: Pick-Up and Twist Lock™ Transfer Copings are both available in the external hex design and three EP® (Emergence Profile) Diameters. The patented Twist Lock Design provides a more accurate transfer of the implant hex compared to other transfer (closed tray) techniques. The unique Twist Lock Feature provides a series of undercuts to guide the coping into the impression for stability. As a result, the copings lock into orientation grooves upon clockwise rotation, thereby allowing a tactile sensation of resistance that ensures an accurate hex transfer.



- Precise Abutment Placement: The Asyst Abutment Placement Tool provides fingertip control for fast and easy abutment delivery. The patented packaging design makes abutment placement easier because the abutment is delivered sterile from the package directly to the implant site. The system includes the abutment, abutment screw and plastic seating device. The plastic seating device facilitates precise placement of the abutment on the implant, thus reducing chair time. The Asyst Tool is packaged with the Standard and Conical Abutments.

Introduction

Patient Specific Restorations® Overview

ARCHITECH PSR®



Encode® Impression System

The Encode Impression System eliminates the need for an implant-level impression while delivering a Patient Specific Restoration that has the appropriate margin height and natural emergence contours for the patient.

This accuracy is achieved from an impression of the Encode Healing Abutment. Codes embedded on the occlusal surface of the Encode Healing Abutment communicate the collar height, implant hex-orientation, platform diameter and interface (the Certain® Internal Connection or External Hex Connection) of the implant. Because the tissue is healed at the time of impression, the margin is designed to have the appropriate placement and contour. The result is a patient specific, anatomically designed, final Encode Abutment. Available in titanium, titanium nitride coating and zirconia.



CAM StructSURE® Precision Milled Bars And Frameworks

CAM StructSURE Precision Milled Bars are created with the technology to achieve a truly passive fit. These are available in Hader and Dolder® Designs for overdenture bars, primary bars and in fixed hybrid designs. This technology does not require any wax or resin design from the technician. The bars can be made on most major dental implants and abutments. Because these are milled from one solid piece of lightweight titanium, the potential for weakness caused by soldering or laser welded joints is eliminated. You receive a completed superstructure ready for prosthesis processing. No polishing or retention creation necessary. BIOMET 3i can even tap holes for attachments.





















Copy Milled Bars are also available for those who prefer to design a bar or framework in resin pattern to the patient's specifications.

Note: Please ensure that as many implants as necessary are used for a fully stable restoration.

Introduction


Patient Specific Restorations® Overview

Available CAM StructSURE® Precision Milled Bar Designs


<p>Hybrid Design #1</p>   <ul style="list-style-type: none"> • Fixed prosthesis • Metal lingual • Low buccal finish line 	<p>Hybrid Design #2</p>   <ul style="list-style-type: none"> • Fixed prosthesis • Designed for easy hygiene • Metal lingual • Buccal and lingual finish lines 	<p>Wrap Around Bar</p>  <ul style="list-style-type: none"> • Fixed prosthesis • Acrylic resin wraps around the bar 	<p>Canada Bar</p>   <ul style="list-style-type: none"> • Fixed hybrid bar • Removable prosthesis engages bar
<p>Dolder® Eggshape</p>   <ul style="list-style-type: none"> • Removable overdenture design • Clips allow for anterior/posterior rotation of the denture 	<p>Dolder U Shape</p>   <ul style="list-style-type: none"> • Removable overdenture design with clips for more rigid fit • Clips allow for anterior/posterior rotation of the denture • Provides lateral stability to denture 	<p>Hader Bar</p>   <ul style="list-style-type: none"> • Removable overdenture design with clips that engage undercuts • Provides some lateral stability • 4mm between implants is needed for clips 	
<p>Primary Bar</p>   <ul style="list-style-type: none"> • Most secure removable overdenture design • May be used with attachments or secondary casting • Bar can be designed with a 2° – 6° taper 	<p>Combination Primary With Hader Or Dolder</p>   <ul style="list-style-type: none"> • Combines a milled bar with Hader or Dolder Designs • Excellent lateral stability • Bar can be designed with a 2° – 6° taper 	<p>Copy Milled</p>  <ul style="list-style-type: none"> • Fixed or removable bar prosthesis • Framework for fixed prosthesis • Technician fabricated resin pattern for porcelain or acrylic bonded to titanium • Must fall within existing design parameters 	

Restorative Products Flow Chart

Cement-Retained Restoration Details

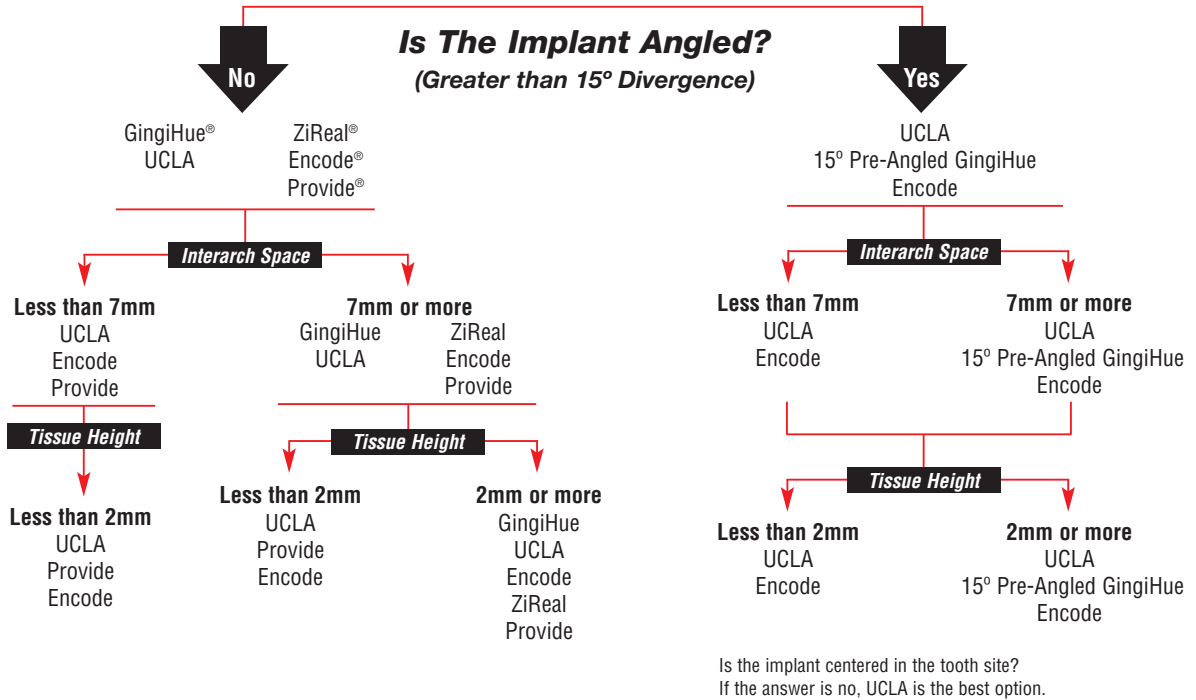

Screw-Retained Restoration Details

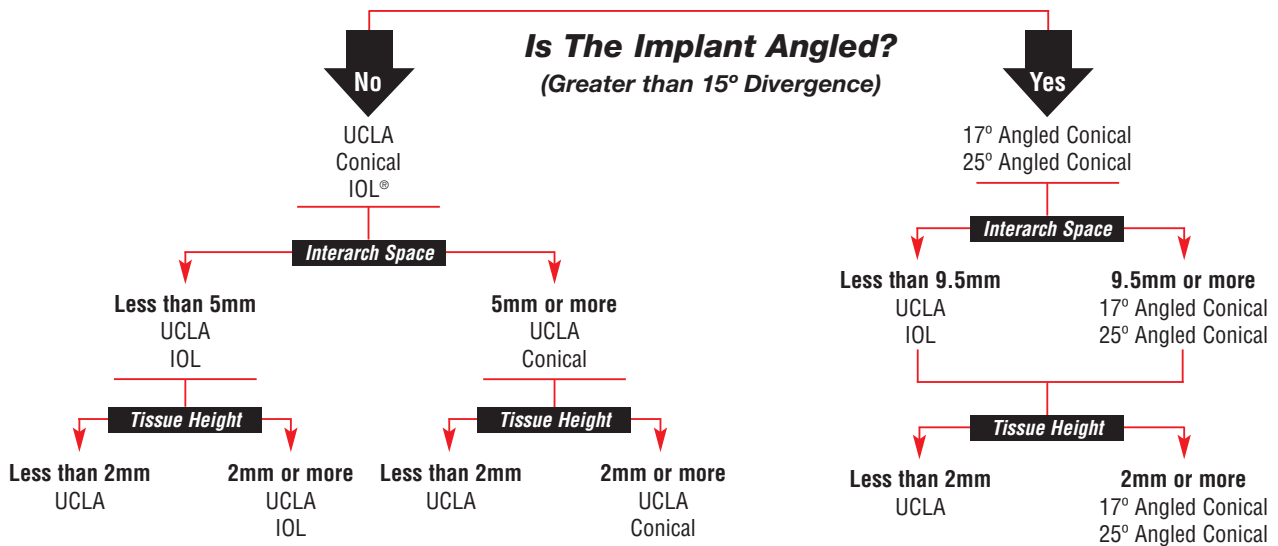

Is the implant centered in the tooth site? If the answer is no, UCLA is the best option.

Provide® Abutment Selection Guide

	Blue	Blue	Yellow	Green	Yellow	Green
	 a = 4.1mm c = 4mm d = 4.8mm	 a = 4.1mm c = 5.5mm d = 4.8mm	 a = 5mm c = 4mm d = 6.5mm	 a = 6mm c = 4mm d = 6.5mm	 a = 5mm c = 5.5mm d = 6.5mm	 a = 6mm c = 5.5mm d = 6.5mm
Abutments	IPA4140 IPA4240 IPA4340 IPA4440	IPA4155 IPA4255 IPA4355 IPA4455	IPA5140 IPA5240 IPA5340 IPA5440	IPA6140 IPA6240 IPA6340 IPA6440	IPA5155 IPA5255 IPA5355 IPA5455	IPA6155 IPA6255 IPA6355 IPA6455
Screws	IUNIHG	IUNIHG	IUNIHG	IUNIHG	IUNIHG	IUNIHG
Protection Caps	PPC484	PPC485	PPC654	PPC654	PPC655	PPC655
Impression Copings	PIC484 <i>Non-Prepared</i> PIC484H <i>Prepared</i>	PIC485 <i>Non-Prepared</i> PIC485H <i>Prepared</i>	PIC654 <i>Non-Prepared</i> PIC654H <i>Prepared</i>	PIC654 <i>Non-Prepared</i> PIC654H <i>Prepared</i>	PIC655 <i>Non-Prepared</i> PIC655H <i>Prepared</i>	PIC655 <i>Non-Prepared</i> PIC655H <i>Prepared</i>
Laboratory Analogs	PAA484 <i>Non-Prepared</i> PAAP48 <i>Prepared</i>	PAA485 <i>Non-Prepared</i> PAAP48 <i>Prepared</i>	PAA654 <i>Non-Prepared</i> PAAP65 <i>Prepared</i>	PAA654 <i>Non-Prepared</i> PAAP65 <i>Prepared</i>	PAA655 <i>Non-Prepared</i> PAAP65 <i>Prepared</i>	PAA655 <i>Non-Prepared</i> PAAP65 <i>Prepared</i>
Waxing Sleeves	PWS48S <i>Single Unit</i> PWS48M <i>Multi-Unit</i>	PWS48S <i>Single Unit</i> PWS48M <i>Multi-Unit</i>	PWS65S <i>Single Unit</i> PWS65M <i>Multi-Unit</i>	PWS65S <i>Single Unit</i> PWS65M <i>Multi-Unit</i>	PWS65S <i>Single Unit</i> PWS65M <i>Multi-Unit</i>	PWS65S <i>Single Unit</i> PWS65M <i>Multi-Unit</i>
Temporary Cylinders	PUA48S <i>Single Unit</i> PUA48M <i>Multi-Unit</i>	PUA48S <i>Single Unit</i> PUA48M <i>Multi-Unit</i>	PUA65S <i>Single Unit</i> PUA65M <i>Multi-Unit</i>	PUA65S <i>Single Unit</i> PUA65M <i>Multi-Unit</i>	PUA65S <i>Single Unit</i> PUA65M <i>Multi-Unit</i>	PUA65S <i>Single Unit</i> PUA65M <i>Multi-Unit</i>

* b: collar height selection depends on tissue depth

Cement-Retained Restorations


Certain® Internal Connection


Provide® Abutments

Indications:

- Single and multi-unit porcelain fused to metal restorations
- Fixed margin abutments
- Snap-on impression components
- Maximum angulation correction of 10°
- Minimum interarch space of 7mm

Material:
Titanium Alloy


4.1mm Seating Surface					
Emergence Profile	Collar Height	Post Height	Item Numbers		
			Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
4.8mm	1.0mm	4.0mm	PAK4140*	PRK484**	IPA4140
4.8mm	2.0mm	4.0mm	PAK4240*	PRK484**	IPA4240
4.8mm	3.0mm	4.0mm	PAK4340*	PRK484**	IPA4340
4.8mm	4.0mm	4.0mm	PAK4440*	PRK484**	IPA4440
4.8mm	1.0mm	5.5mm	PAK4155*	PRK485**	IPA4155
4.8mm	2.0mm	5.5mm	PAK4255*	PRK485**	IPA4255
4.8mm	3.0mm	5.5mm	PAK4355*	PRK485**	IPA4355
4.8mm	4.0mm	5.5mm	PAK4455*	PRK485**	IPA4455



5.0mm Seating Surface					
Emergence Profile	Collar Height	Post Height	Item Numbers		
			Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
6.5mm	1.0mm	4.0mm	PAK5140*	PRK654**	IPA5140
6.5mm	2.0mm	4.0mm	PAK5240*	PRK654**	IPA5240
6.5mm	3.0mm	4.0mm	PAK5340*	PRK654**	IPA5340
6.5mm	4.0mm	4.0mm	PAK5440*	PRK654**	IPA5440
6.5mm	1.0mm	5.5mm	PAK5155*	PRK655**	IPA5155
6.5mm	2.0mm	5.5mm	PAK5255*	PRK655**	IPA5255
6.5mm	3.0mm	5.5mm	PAK5355*	PRK655**	IPA5355
6.5mm	4.0mm	5.5mm	PAK5455*	PRK655**	IPA5455



6.0mm Seating Surface					
Emergence Profile	Collar Height	Post Height	Item Numbers		
			Abutment Placement Kit	Abutment Restorative Kit	Abutment Only
6.5mm	1.0mm	4.0mm	PAK6140*	PRK654**	IPA6140
6.5mm	2.0mm	4.0mm	PAK6240*	PRK654**	IPA6240
6.5mm	3.0mm	4.0mm	PAK6340*	PRK654**	IPA6340
6.5mm	4.0mm	4.0mm	PAK6440*	PRK654**	IPA6440
6.5mm	1.0mm	5.5mm	PAK6155*	PRK655**	IPA6155
6.5mm	2.0mm	5.5mm	PAK6255*	PRK655**	IPA6255
6.5mm	3.0mm	5.5mm	PAK6355*	PRK655**	IPA6355
6.5mm	4.0mm	5.5mm	PAK6455*	PRK655**	IPA6455




*Abutment Placement Kit includes the Provide Abutment, Protection Cap and Certain® Gold-Tite® Hexed Screw IUNIHG.
 **Abutment Restorative Kit includes Impression Coping, Impression Coping w/Holes, Waxing Sleeve (single-unit), Waxing Sleeve (multi-unit) and Non-Prepared Analog.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations


Certain® Internal Connection

Provide® Components

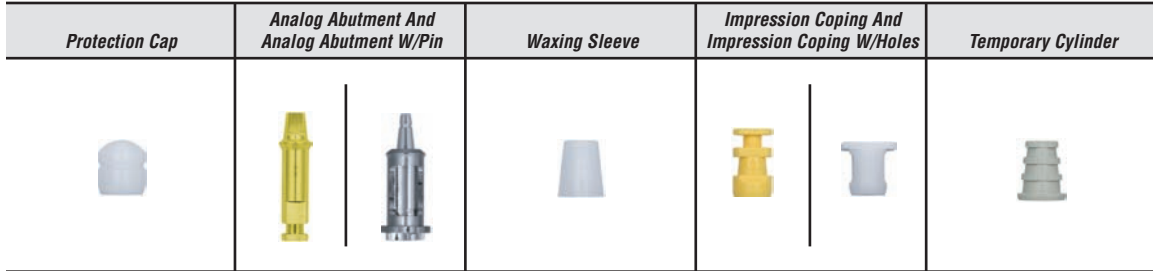

Description	4.0mm Post Height		5.5mm Post Height		
	Emergence Profile	4.8	6.5	4.8	6.5
Protection Cap		PPC484	PPC654	PPC485	PPC655
Impression Coping (Unprepared)		▶ PIC484	▶ PIC654	▶ PIC485	▶ PIC655
Impression Coping W/Holes (Prepared)		PIC484H	PIC654H	PIC485H	PIC655H
Abutment Analog (Unprepared)		▶ PAA484	▶ PAA654	▶ PAA485	▶ PAA655
Abutment Analog W/Pin (Prepared)		PAAP48	PAAP65	PAAP48	PAAP65
Abutment Screw		IUNIHG*, IUNIHT			
Waxing Sleeve	single-unit ↓	PWS48S	PWS65S	PWS48S	PWS65S
	multi-unit ↓	PWS48M	PWS65M	PWS48M	PWS65M
Temporary Cylinder	single-unit ↓	PUA48S	PUA65S	PUA48S	PUA65S
	multi-unit ↓	PUA48M	PUA65M	PUA48M	PUA65M

*Recommended

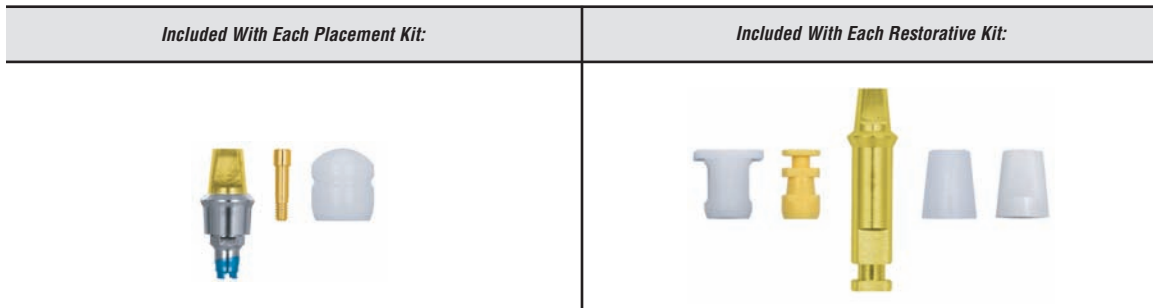

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection


GingiHue® Posts

Indications:

- Single and multi-unit porcelain fused to metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 6mm

Material:

Titanium Alloy

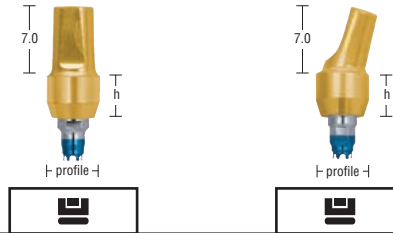

Prep-Tite® Cap For Straight GingiHue Posts



3.4mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
3.8mm	2.0mm	IMAP32G	IMPAP32G	5mm	PTC345
3.8mm	4.0mm	IMAP34G	IMPAP34G	5mm	PTC345

4.1mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
5.0mm	2.0mm	IAPP452G	IPAP452G	5mm	PTC455
5.0mm	4.0mm	IAPP454G	IPAP454G	5mm	PTC455
6.0mm	2.0mm	IAPP462G	IPAP462G	5mm	PTC465
6.0mm	4.0mm	IAPP464G	IPAP464G	5mm	PTC465
7.5mm	2.0mm	IAPP472G	IPAP472G	5mm	PTC475
7.5mm	4.0mm	IAPP474G	IPAP474G	5mm	PTC475

5.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
5.0mm	2.0mm	IWPP552G	IPAP552G	5mm	PTC555
5.0mm	4.0mm	IWPP554G	IPAP554G	5mm	PTC555
6.0mm	2.0mm	IWPP562G	IPAP562G	5mm	PTC465
6.0mm	4.0mm	IWPP564G	IPAP564G	5mm	PTC465
7.5mm	2.0mm	IWPP572G	IPAP572G	5mm	PTC475
7.5mm	4.0mm	IWPP574G	IPAP574G	5mm	PTC475

6.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
6.0mm	2.0mm	IWPP662G	IPAP662G	5mm	PTC665
6.0mm	4.0mm	IWPP664G	IPAP664G	5mm	PTC665
7.5mm	2.0mm	IWPP672G	IPAP672G	5mm	PTC475
7.5mm	4.0mm	IWPP674G	IPAP674G	5mm	PTC475


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

GingiHue® Post Components

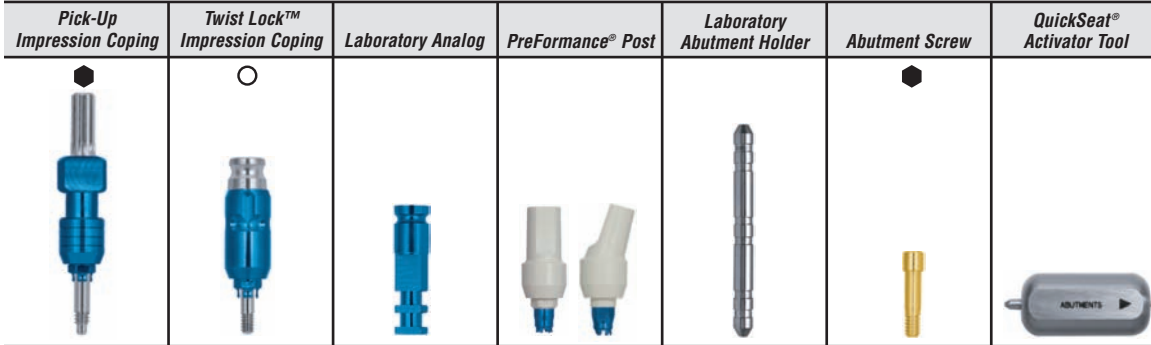

= Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N
 = Requires the use of Impression Coping Driver IC000

Description	3.4mm		4.1mm				5.0mm				6.0mm			
	Emergence Profile	3.4	3.8	4.1	5.0	6.0	7.5	5.0	5.6	6.0	7.5	6.0	6.8	7.5
Pick-Up Impression Coping	IMIC30	IMIC33	IIIC41, IIIC42*	IIIC12	IIIC60	IIIC75	IWIP50	IWIP55	IWIP56	IWIP57	IWIP60	IWIP66	IWIP67	
Twist Lock Impression Coping	N/A	N/A	IIIC44	IIIC45	IIIC46	IIIC47	IWIT50	IWIT55	IWIT56	IWIT57	IWIT60	IWIT66	IWIT67	
Laboratory Analog	IMMILA	IMMILA	IILA20	IILA20	IILA20	IILA20	IILAW5	IILAW5	IILAW5	IILAW5	IILAW6	IILAW6	IILAW6	
Laboratory Abutment Holder	ILTAH57													
Abutment Screw	IUNIHG**, IUNIHT													
Hex Try-In Screw (5-pack)	IUNITS													
QuickSeat Activator Tool	IQSA01													
PreFormance Post	See page 23													

*Non-Hexed
**Recommended

Certain Internal Connection

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection


ZiReal® Posts


Indications:

- Single and multi-unit all ceramic restorations
- Preparable to follow gingival contours
- Minimum interarch space of 6mm
- Aesthetic restorations when tissue is limited
- Maximum angulation of 10°

Material:

Zirconia Ceramic With A Titanium Alloy Interface

4.1mm Seating Surface		
Emergence Profile	Collar Height	Item Numbers
5.0mm	4.0mm	ICAP454*
6.0mm	4.0mm	ICAP464*
5.0mm Seating Surface		
Emergence Profile	Collar Height	Item Numbers
6.0mm	4.0mm	IWCAP564*
7.5mm	4.0mm	IWCAP574*



*Includes Certain ZiReal Gold-Tite® Screw (IZSHG) and ZiReal Try-In Screw (IZIRTS).


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

ZiReal® Post Components

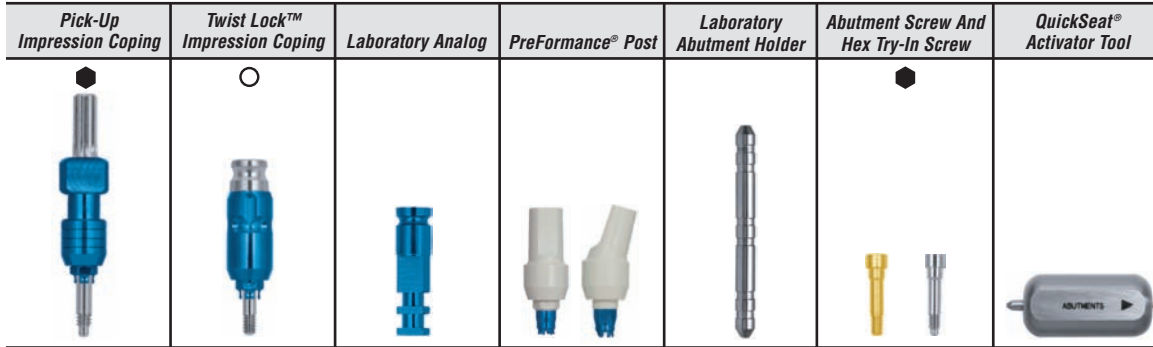

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

○ = Requires the use of Impression Coping Driver **ICD00**

Description	4.1mm				5.0mm				
	Emergence Profile	4.1	5.0	6.0	7.5	5.0	5.6	6.0	7.5
Pick-Up Impression Coping	IIC41, IIC42*	IIC12	IIC60	IIC75	IWIP50	IWIP55	IWIP56	IWIP57	
Twist Lock Impression Coping	IIC44	IIC45	IIC46	IIC47	IWIT50	IWIT55	IWIT56	IWIT57	
Laboratory Analog	IILA20	IILA20	IILA20	IILA20	IILAW5	IILAW5	IILAW5	IILAW5	
Laboratory Abutment Holder	ILTAH57								
Abutment Screw (included)	IZSHG								
Hex Try-In Screw (included)	IZIRTS								
QuickSeat Activator Tool	IQSA01								
PreFormance Post	See page 23								

*Non-Hexed

Certain Internal Connection

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

UCLA Abutments

Indications:


- Laboratory fabricated custom abutments
- Single and multi-unit restorations
- Minimum interarch space of 6mm
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	IMUCG1C
4.1mm Seating Surface	
Gold (Hexed)	IGUCA1C
Gold Standard ZR™ (Hexed)	N/A
Castable (Hexed)	N/A
Castable (Hexed) 25PK	N/A
5.0mm Seating Surface	
Gold (Hexed)	IWGA51C
Gold Standard ZR (Hexed)	N/A
Castable (Hexed)	N/A
6.0mm Seating Surface	
Gold (Hexed)	IWGA61C
Gold Standard ZR (Hexed)	N/A
Castable (Hexed)	N/A




All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

Certain® Internal Connection

UCLA Abutment Components

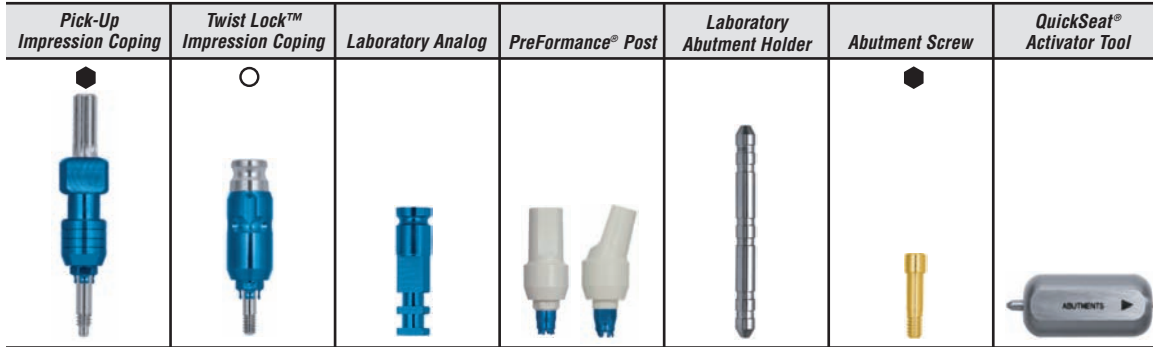

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
 = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm			4.1mm			5.0mm			6.0mm			
	3.4	3.8	4.1	5.0	6.0	7.5	5.0	5.6	6.0	7.5	6.0	6.8	7.5
Pick-Up Impression Coping	IMIC30	IMIC33	IIIC41, IIIC42*	IIIC12	IIIC60	IIIC75	IWIP50	IWIP55	IWIP56	IWIP57	IWIP60	IWIP66	IWIP67
Twist Lock Impression Coping	N/A	N/A	IIIC44	IIIC45	IIIC46	IIIC47	IWIT50	IWIT55	IWIT56	IWIT57	IWIT60	IWIT66	IWIT67
Laboratory Analog	IMMILA	IMMILA	IILA20	IILA20	IILA20	IILA20	IILAW5	IILAW5	IILAW5	IILAW5	IILAW6	IILAW6	IILAW6
Laboratory Abutment Holder	ILTAH57												
Abutment Screw	IUNIHG**, IUNIHT												
Hex Try-In Screw (5-pack)	IUNITS												
QuickSeat Activator Tool	IQSA01												
PreFormance Post	See page 23												

*Non-Hexed
**Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ °K at 500°C

An alloy with a CTE of 10⁻⁶°K at 500°C is recommended.

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

UCLA Abutments

Indications:


- Single and multi-unit restorations
- Minimum interarch space of 4mm
- For aesthetic restorations when tissue is limited

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	IMUCG1C
Gold (Non-Hexed)	IMUCG2C
Gold (Non-Hexed)	IMUCG2T**
Castable (Non-Hexed)	IMUCC2C*
Castable (Non-Hexed)	IMUCC2T**
4.1mm Seating Surface	
Gold (Hexed)	IGUCA1C
Gold (Non-Hexed)	IGUCA2C*
Gold (Non-Hexed)	IGUCA2T**
Gold Standard ZR™ (Hexed)	N/A
Castable (Hexed)	N/A
Castable (Non-Hexed)	IUNAB2C*
Castable (Non-Hexed)	IUNAB2T**
Castable (Hexed) 25PK	N/A
Castable (Non-Hexed) 25PK	N/A
5.0mm Seating Surface	
Gold (Hexed)	IWGA51C
Gold (Non-Hexed)	IWGA52C*
Gold (Non-Hexed)	IWGA52T**
Gold Standard ZR (Hexed)	N/A
Castable (Hexed)	N/A
Castable (Non-Hexed)	IWPC52C*
Castable (Non-Hexed)	IWPC52T**
6.0mm Seating Surface	
Gold (Hexed)	IWGA61C
Gold (Non-Hexed)	IWGA62C*
Gold (Non-Hexed)	IWGA62T**
Gold Standard ZR (Hexed)	N/A
Castable (Hexed)	N/A
Castable (Non-Hexed)	IWPC62C*
Castable (Non-Hexed)	IWPC62T**

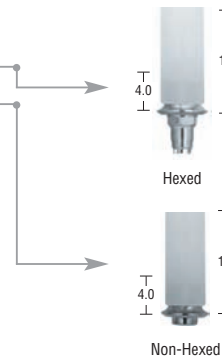

*Large Diameter Gold-Tite® Screw Included.
 **Large Diameter Ti Screw Included


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

UCLA Abutment Cylinder Components

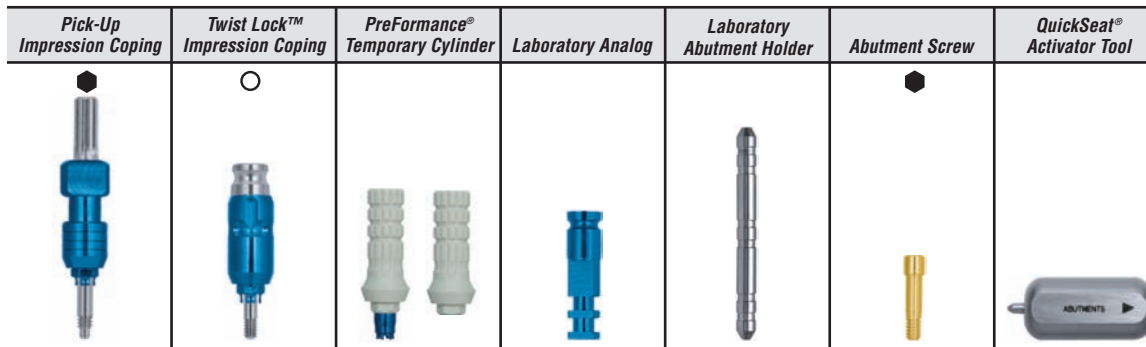

= Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

 = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm		4.1mm				5.0mm			6.0mm				
	Emergence Profile	3.4	3.8	4.1	5.0	6.0	7.5	5.0	5.6	6.0	7.5	6.0	6.8	7.5
Pick-Up Impression Coping	IMIC30	IMIC33	IIIC41, IIIC42*	IIIC12	IIIC60	IIIC75	IWIP50	IWIP55	IWIP56	IWIP57	IWIP60	IWIP66	IWIP67	
Twist Lock Impression Coping	N/A	N/A	IIIC44	IIIC45	IIIC46	IIIC47	IWIT50	IWIT55	IWIT56	IWIT57	IWIT60	IWIT66	IWIT67	
Laboratory Analog	IMMILA		IILA20				IILAW5			IILAW6				
Laboratory Holder	ILTAH57													
PreFormance Temp. Cylinder	hexed ▶	N/A	IMPFTC34	IPFTC41				IWPFTC51			IWPFTC61			
	non-hexed ▶	N/A	IMPFTC32	IPFTC42				IWPFTC52			IWPFTC62			
Temporary Cylinder	hexed ▶	N/A	IMMTCS1	IITCS41				IWTCS51			IWTCS61			
	non-hexed ▶	N/A	N/A	IITCS42				IWTCS52			IWTCS62			
Abutment Screw	Hexed: IUNIHT, IUNIHG**, Non-Hexed: ILRGHG**, ILRGHT													
Hex Try-In Screw (5-pack)	IUNITS (for hexed only)													
QuickSeat Activator Tool	IQSA01													

*Non-Hexed
 **Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ °K at 500°C

An alloy with a CTE of 10⁻⁶°K at 500°C is recommended.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection


Low Profile Abutments

Indications:

- Single and multi-unit screw-retained restorations
- Minimum interarch space of 7.5mm
- Minimum tissue height of 1mm
- Angle correction up to 30°

Material:

Titanium Alloy

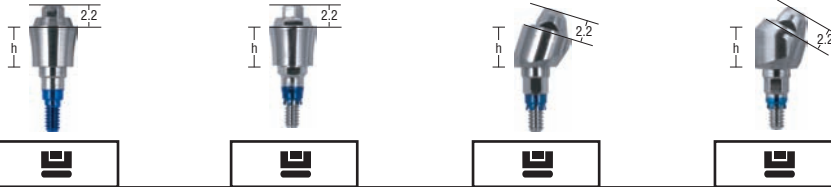

3.4mm Seating Surface		Item Numbers			
Collar Height	Straight (One Piece)	Straight (Two Piece)	17° Pre-Angled	30° Pre-Angled	
1.0mm	ILPC341U	ILPC341	N/A	N/A	
2.0mm	ILPC342U	ILPC342	ILPAC3217	N/A	
3.0mm	ILPC343U	ILPC343	N/A	ILPAC3330	
4.0mm	ILPC344U	ILPC344	ILPAC3417	N/A	
5.0mm	N/A	N/A	N/A	ILPAC3530	

4.1mm Seating Surface		Item Numbers			
Collar Height	Straight (One Piece)	Straight (Two Piece)	17° Pre-Angled	30° Pre-Angled	
1.0mm	ILPC441U	ILPC441	N/A	N/A	
2.0mm	ILPC442U	ILPC442	ILPAC4217	N/A	
3.0mm	ILPC443U	ILPC443	N/A	ILPAC4330	
4.0mm	ILPC444U	ILPC444	ILPAC4417	N/A	
5.0mm	N/A	N/A	N/A	ILPAC4530	

5.0mm Seating Surface		Item Numbers			
Collar Height	Straight (One Piece)	Straight (Two Piece)	17° Pre-Angled	30° Pre-Angled	
1.0mm	ILPC541U	ILPC541	N/A	N/A	
2.0mm	ILPC542U	ILPC542	ILPAC5217	N/A	
3.0mm	ILPC543U	ILPC543	N/A	ILPAC5330	
4.0mm	ILPC544U	ILPC544	ILPAC5417	N/A	
5.0mm	N/A	N/A	N/A	ILPAC5530	











All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

Low Profile Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Healing Cap	Gold And Castable Cylinder
				
QuickBridge®	Temporary Cylinder	Polishing Protector	Retaining Screw	Driver And Driver Tip
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

○ = Requires the use of Impression Coping Driver ICD00

Description		4.8mm Restorative Platform
Pick-Up Impression Coping	hexed ↓ non-hexed ↓	LPCPIC1 LPCPIC2
Twist Lock Impression Coping	hexed ↓ non-hexed ↓	LPCTIC1 LPCTIC2
QuickBridge Impression Coping		LPCRIC
Laboratory Analog		LPCLA
Temporary Cylinder	hexed ↓ non-hexed ↓	LPCTC1 LPCTC2
Healing Cap		LPCHC
PreFormance Temp. Cylinder	hexed ↓ non-hexed ↓	LPCPTC1 LPCPTC2
QuickBridge		LPCQB
QuickBridge Replacement Cap		LPCQBCAP
Distal Extension		LPCDE
Gold Cylinder	hexed ↓ non-hexed ↓	LPCGC1 LPCGC2
Castable Cylinder	hexed ↓ non-hexed ↓	LPCCC1 LPCCC2
Laser Weld Cylinder		LPCTUCA
Waxing Screw		LPCWS
Retaining Screw		LPCGSH, LPCTSH
Lapping Tool		LPCAMI
Polishing Protector		LPCPP

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection


Immediate Occlusal Loading (IOL®) Abutments*


Indications:

- Multi-unit porcelain fused to metal restorations
- Minimum interarch space of 6mm
- Minimum tissue height of 2mm

Material:

Titanium Alloy

4.1mm Seating Surface		
Emergence Profile	Collar Height	Item Numbers
4.5mm	2.0mm	IIOL20S
4.5mm	3.0mm	IIOL30S
4.5mm	4.0mm	IIOL40S
4.5mm	5.5mm	IIOL55S
4.5mm	7.0mm	IIOL70S



Uses **PAD00** (17mm), **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip

*Indications: For surgical placement in the upper or lower jaw to provide a means for prosthetic attachment in single tooth restorations and in partially or fully edentulous spans with multiple single teeth, or as a terminal or intermediary abutment for fixed or removable bridgework and to retain overdentures.

In addition, when a minimum of 4 implants, ≥ 10mm in length, are placed in the mandible and splinted in the anterior region, immediate loading is indicated.

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

IOL® Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Temporary Cylinder	Gold Cylinder
Healing Cap	Polishing Protector	Driver And Driver Tip	Retaining And Waxing Screw	
				= Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

Description	4.1mm
Emergence Profile	4.5
Pick-Up Impression Coping	IOLPIC
Twist Lock Impression Coping	IOLTIC
Laboratory Analog	IOLLAS
Temporary Cylinder	IOLTC
Gold Cylinder	IOLGC
Healing Cap	IOLHC
Polishing Protector	IOLPP
Driver	PAD00, PAD24
Driver Tip	RASA3
Retaining Screw	GSH30, GSH70
Waxing Screw	WSK10, WSK15

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

Conical Abutments

Indications:

- Single and multi-unit porcelain fused to metal restorations
- Minimum interarch space of 7mm
- Minimum tissue height of 2mm

Material:

Titanium Alloy



3.4mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)*	Item Numbers (25° Pre-Angled)*
3.4mm	1.0mm	IMCA31	N/A	N/A
3.4mm	2.0mm	IMCA32	N/A	N/A
3.4mm	3.0mm	IMCA33	N/A	N/A
3.4mm	4.0mm	IMCA34	N/A	N/A

4.1mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
5.0mm	1.0mm	ICA001	N/A	N/A
5.0mm	2.0mm	ICA002	IAC4217	IAC4225
5.0mm	3.0mm	ICA003	N/A	N/A
5.0mm	4.0mm	ICA004	IAC4417	IAC4425
5.0mm	5.5mm	ICA055	N/A	N/A

5.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
5.0mm	1.0mm	IWCA51	N/A	N/A
5.0mm	2.0mm	IWCA52	N/A	N/A
5.0mm	3.0mm	IWCA53	N/A	N/A
5.0mm	4.0mm	IWCA54	N/A	N/A
5.0mm	5.5mm	IWCA55	N/A	N/A

6.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
6.0mm	1.0mm	IWCA61**	N/A	N/A
6.0mm	2.0mm	IWCA62	N/A	N/A
6.0mm	3.0mm	IWCA63	N/A	N/A
6.0mm	4.0mm	IWCA64	N/A	N/A
6.0mm	5.5mm	IWCA65	N/A	N/A

Uses **PAD00** (17mm) or **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip.

*It is recommended that small diameter implants not be restored with angled abutments in the molar region.











**Requires Gold-Tite® Retaining Screw (GSH20)

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

Certain® Internal Connection

Conical Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Healing Cap	Gold And Castable Cylinder
				
QuickBridge®	Temporary Cylinder	Polishing Protector	Retaining Screw	Driver And Driver Tip
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

○ = Requires the use of Impression Coping Driver ICD00

Description	Emergence Profile	3.4mm			4.1mm			5.0mm			6.0mm	
		3.8	5.0	6.0	7.5	5.0	6.0	7.5	6.0	7.5		
Pick-Up Impression Coping	single-unit ↓	MEC33	CNRC	CSQN6	CSQN7	CNRC	CSQN6	CSQN7	WCP661	WCP671		
	multi-unit ↓	N/A	CSQI7	CSQ06	CSQ07	CSQI7	CSQ06	CSQ07	WCP662	N/A		
Twist Lock Impression Coping	single-unit ↓	N/A	N/A	N/A	N/A	N/A	N/A	N/A	WCT661	WCT671		
	multi-unit ↓	N/A	CIC55	CIC56	CIC57	CIC55	CIC56	CIC57	WCT662	WCT672		
Laboratory Analog		MMCLA	CLA20	CLA20	CLA20	CLA20	CLA20	CLA20	WCLA6	WCLA6		
Healing Cap		MHC33	CS250	CS260	CS270	CS250	CS260	CS270	WCS66	WCS67		
Gold Cylinder	single-unit ↓	MCAG1*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG6*	CNRG6*		
	multi-unit ↓	MCAG2*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC6*	CAGC6*		
Castable Cylinder	single-unit ↓	N/A	CNRC5*	CNRC5*	CNRC5*	CNRC5*	CNRC5*	CNRC5*	N/A	N/A		
	multi-unit ↓	N/A	CACC5*	CACC5*	CACC5*	CACC5*	CACC5*	CACC5*	N/A	N/A		
Temporary Cylinder	single-unit ↓	MCTC1*	CNC30*	CNC30*	CNC30*	CNC30*	CNC30*	CNC30*	WCTC60*	N/A		
	multi-unit ↓	MCTC2*	CC300*	CC300*	CC300*	CC300*	CC300*	CC300*	WCTC61*	WCTC671*		
QuickBridge	multi-unit ↓	N/A	QKBRG	QKBRG	QKBRG	QKBRG	QKBRG	QKBRG	N/A	N/A		
Polishing Protector		PPMC1	PPCA3	PPCA3	PPCA3	PPCA3	PPCA3	PPCA3	WCPP6	WCPP6		
Retaining Screw			GSH30, GSH70**							GSH20, GSH30, GSH70**		

*Requires Gold-Tite® Retaining Screw.

**Height of screw may be adjusted to access hole depth.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection

DIEM® Immediate Occlusal Loading (IOL®) Abutments

Indications:


- Multiple implant bar retained and fixed removable overdentures
- Minimum interarch space of 9.2mm
- Maximum angulation of 30°

Material:

Titanium Alloy

Immediate Occlusal Loading:

- Adequate bone quality equal to or greater than Type III
- Bone height equal to or greater than 12mm to allow for a minimum 10mm implant
- Bone width equal to or greater than 6mm to allow for a minimum 4mm diameter implant
- Adequate curvature of the arch and space between mental foramina, to permit proper anterior/posterior spread measurement, will allow functional cantilevers to 1st molar occlusion

4.1mm Seating Surface		
Emergence Profile	Collar Height	Item Numbers
4.5mm	2.0mm	I1OL20S
4.5mm	3.0mm	I1OL30S
4.5mm	4.0mm	I1OL40S
4.5mm	5.5mm	I1OL55S
4.5mm	7.0mm	I1OL70S



Uses PAD00 (17mm), PAD24 (24mm) Abutment Driver or RASA3 Driver Tip

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection

DIEM® Immediate Occlusal Loading (IOL®) Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Temporary Cylinder	Gold Cylinder
Distal Extension	Healing Cap	Polishing Protector	Driver And Driver Tip	Retaining And Waxing Screw

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

Description	4.1mm
Emergence Profile	4.5
Pick-Up Impression Coping	IOLPIC
Twist Lock Impression Coping	IOLTIC
Laboratory Analog	IOLLAS
Temporary Cylinder	IOLTC
Gold Cylinder	IOLGC
Distal Extension	IOLDE
Healing Cap	IOLHC
Polishing Protector	IOLPP
Driver	PAD00, PAD24
Driver Tip	RASA3
Retaining Screw	GSH30, GSH70
Waxing Screw	WSK10, WSK15

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection

Standard Abutments

Indications:

- Multiple implant bar retained and fixed removable overdentures
- Minimum interarch space of 6.5mm
- Maximum divergence of 30°


Material:

Titanium Alloy

4.1mm Seating Surface



Collar Height	Item Numbers
2.0mm	IAB200*
3.0mm	IAB300
4.0mm	IAB400
5.5mm	IAB550
7.0mm	IAB700



Uses **PAD00** (17mm) or **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip.











*Requires Gold-Tite® Retaining Screw (GSH20)

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection

Standard Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Gold Cylinder	Temporary Cylinder
				
Polishing Protector	Healing Cap	Retaining Screw	Driver And Driver Tip	LOCATOR® Bar Attachment
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

○ = Requires the use of Impression Coping Driver ICD00

Description	4.1mm
Emergence Profile	4.5
Pick-Up Impression Coping	SQIC7
Twist Lock Impression Coping	SIC70
Laboratory Analog	SLA20
Gold Cylinder	SGC30**
Chamfered Gold Cylinder	CGC30**
Castable Gold Cylinder	SGC34**
LOCATOR Bar Attachment	LOAB*
LOCATOR Bar Attachment Tap	LOAT
LOCATOR Drill	LOAD
Gold Hader Clip	ORCG1
Plastic Hader Clip	ORCY1
Temporary Cylinder	TC300**
Polishing Protector	PPSA3
Healing Cap	TS250
Retaining Screw	GSH20, GSH30, GSH70***

*Includes LOCATOR Attachment, Housing, Processing Male, Spacer Males, 3 Retention Replacement Males

**Requires Gold-Tite® Retaining Screw (GSH30, GSH70).

***Height of screw may be adjusted to access hole depth.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection


LOCATOR® Abutments


Indications:

- Tissue supported removable overdentures on 2 to 4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants

Material:


Abutment: Titanium Alloy With Titanium Nitride Coating
 Housing: Titanium Alloy
 Males: Nylon

3.4mm Seating Surface		
Collar Height		Item Numbers
1.0mm		IMLOA001
2.0mm		IMLOA002
3.0mm		IMLOA003
4.0mm		IMLOA004
5.0mm		IMLOA005
6.0mm		IMLOA006

4.1mm Seating Surface		
Collar Height		Item Numbers
1.0mm		ILOA001
2.0mm		ILOA002
3.0mm		ILOA003
4.0mm		ILOA004
5.0mm		ILOA005
6.0mm		ILOA006



Included With Each Abutment:

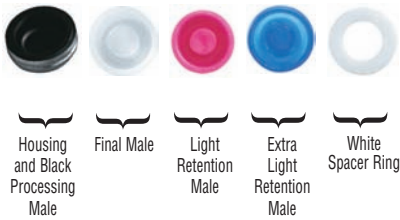





All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

Certain® Internal Connection

LOCATOR® Abutment Components

Impression Coping	Laboratory Analog	Retention Males	Core Tool / Driver And Driver Tip
			

Description	Item Numbers
Impression Coping	LAIC1
Laboratory Analog	LALA1
Extra Light Retention Males (4-pack) - Blue, 1.5lbs/680g	LAELM
Extended Range Males (4-pack) - Green, 4lbs/1800g	LAERM
Extra Light Retention Extended Range Males - Red, 1.5lbs/680g	LELARM
Replacement Males (4-pack) - White, 5lbs/2250g	LARMS
Light Retention Replacement Males (4-pack) - Pink, 3lbs/1350g	LLRMS
Replacement Housing	LOAH
Replacement Housing Kit	LORHK*
Core Tool/Abutment Driver	LCTDR1
Driver Tip 24mm(L)	LOADT4
Driver Tip 30mm(L)	LOADT9
1.25mm/.050in. Driver Tip 24mm(L) - used with LCTDR1	RASH4
1.25mm/.050in. Driver Tip 30mm(L) - used with LCTDR1	RASH9
LOCATOR Bar Attachment	LOAB
LOCATOR Bar Attachment Tap	LOAT
LOCATOR Bar Attachment Drill	LOAD

*Included With **LORHK**
Replacement Housing Kit:



Certain Internal Connection

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

Certain® Internal Connection


PreFormance® Posts

Indications:

- Single and multiple unit provisional cement-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft tissue healing of single and multiple unit restorations of integrated implants

Material:

PEEK: Titanium Alloy Connection

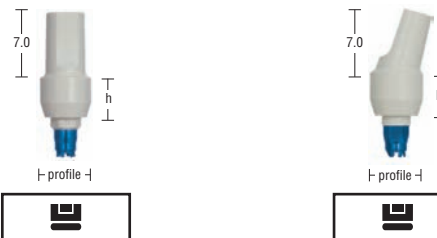

3.4mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
3.8mm	4.0mm	IMPFP34	IMPAPF34
3.8mm	6.0mm	IMPFP36	IMPAPF36
4.1mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5.0mm	4.0mm	IPFP454	IPAPF454
5.0mm	6.0mm	IPFP456	IPAPF456
5.0mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
5.0mm	4.0mm	IWPFP554	IPAPF554
5.0mm	6.0mm	IWPFP556	IPAPF556
6.0mm Seating Surface			
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)
6.0mm	4.0mm	IWPFP664	IPAPF664
6.0mm	6.0mm	IWPFP666	IPAPF666

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

Certain® Internal Connection

PreFormance® Temporary Cylinders


Indications:

- Single and multiple unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multiple unit restorations of integrated implants for guided tissue healing

Material:

PEEK: Titanium Alloy Connection

Description	Item Numbers
3.4mm Seating Surface	
Hexed	IMPFTC34
Non-Hexed	IMPFTC32
4.1mm Seating Surface	
Hexed	IPFTC41
Non-Hexed	IPFTC42
5.0mm Seating Surface	
Hexed	IWPFTC51
Non-Hexed	IWPFTC52
6.0mm Seating Surface	
Hexed	IWPFTC61
Non-Hexed	IWPFTC62



Certain Internal Connection

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection



GingiHue® Posts

Indications:

- Single and multi-unit porcelain fused to metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 6mm

Material:

- Straight Post (Commercially Pure Titanium)
- Pre-Angled Post (Titanium Alloy)



Prep-Tite® Cap For Straight GingiHue Posts



3.4mm Seating Surface					
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
3.8mm	2.0mm	MAP32G	MPAP32G	7mm	PTC347
3.8mm	4.0mm	MAP34G	MPAP34G	7mm	PTC347
4.1mm Seating Surface					
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
5.0mm	2.0mm	APP452G	PAP452G	7mm	PTC457
5.0mm	4.0mm	APP454G	PAP454G	7mm	PTC457
6.0mm	2.0mm	APP462G	PAP462G	7mm	PTC467
6.0mm	4.0mm	APP464G	PAP464G	7mm	PTC467
7.5mm	2.0mm	APP472G	PAP472G	7mm	PTC477
7.5mm	4.0mm	APP474G	PAP474G	7mm	PTC477
5.0mm Seating Surface					
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
5.0mm	2.0mm	WPP552G	PAP552G	7mm	PTC557
5.0mm	4.0mm	WPP554G	PAP554G	7mm	PTC557
6.0mm	2.0mm	WPP562G	PAP562G	7mm	PTC467
6.0mm	4.0mm	WPP564G	PAP564G	7mm	PTC467
7.5mm	2.0mm	WPP572G	PAP572G	7mm	PTC477
7.5mm	4.0mm	WPP574G	PAP574G	7mm	PTC477
6.0mm Seating Surface					
Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (15° Pre-Angled)	Height	Item Numbers
6.0mm	2.0mm	WPP662G	PAP662G	7mm	PTC667
6.0mm	4.0mm	WPP664G	PAP664G	7mm	PTC667
7.5mm	2.0mm	WPP672G	PAP672G	7mm	PTC477
7.5mm	4.0mm	WPP674G	PAP674G	7mm	PTC477


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

GingiHue® Post Components

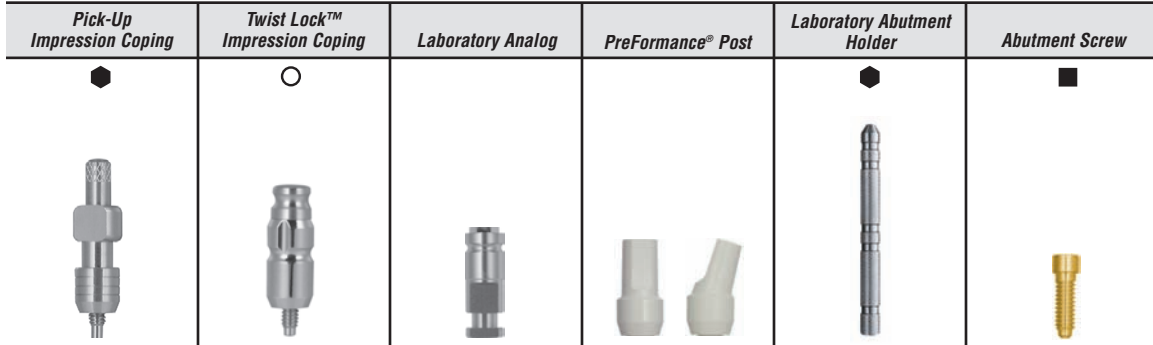

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

■ = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

○ = Requires the use of Impression Coping Driver **ICD00**

Description	3.4mm	4.1mm			5.0mm			6.0mm		
	Emergence Profile	3.8	5.0	6.0	7.5	5.0	6.0	7.5	6.0	7.5
Pick-Up Impression Coping	MIC33	IIC12	IIC60	IIC75		WIP55	WIP56	WIP57	WIP66	WIP67
Twist Lock Impression Coping	N/A	IIC45	IIC46	IIC47		WIT55	WIT56	WIT57	WIT66	WIT67
Laboratory Analog	MMILA	ILA20	ILA20	ILA20		ILAW5	ILAW5	ILAW5	ILAW6	ILAW6
Laboratory Abutment Holder	LTAH5	LTAH7	LTAH7	LTAH7		LTAH7	LTAH7	LTAH7	LTAH7	LTAH7
Abutment Screw	UNISG* [*] ; UNIHG, UNIHT									
Square Try-In Screw (5-pack)	MUNITS	UNITS								
PreFormance Post	See page 47									

*Non-Hexed
**Recommended

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

ZiReal® Posts

Indications:

- Single and multi-unit all ceramic restorations
- Preparable to follow gingival contours
- Minimum interarch space of 6mm
- Aesthetic restorations when tissue is limited
- Maximum angulation of 10°

Material:

Zirconia Ceramic With A Titanium Alloy Interface

4.1mm Seating Surface		Item Numbers
Emergence Profile	Collar Height	
5.0mm	4.0mm	CAP454
6.0mm	4.0mm	CAP464
5.0mm Seating Surface		Item Numbers
Emergence Profile	Collar Height	
6.0mm	4.0mm	WCAP564
7.5mm	4.0mm	WCAP574




All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations


External Hex Connection

ZiReal® Post Components

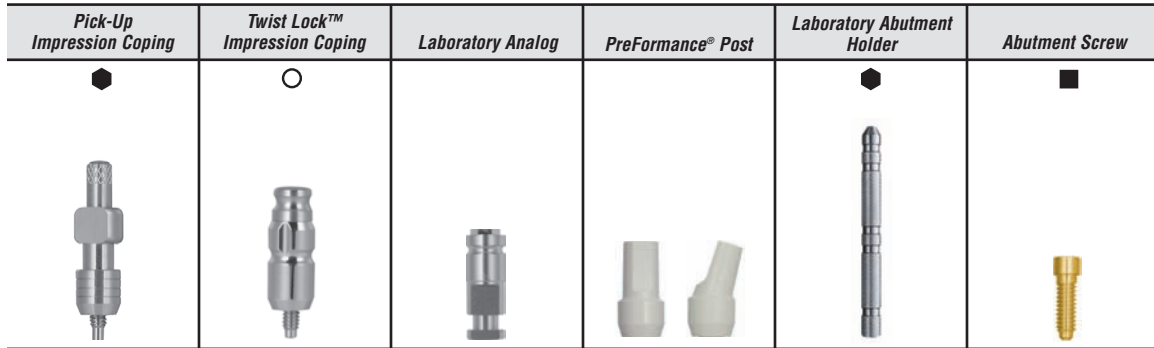

 = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

 = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

 = Requires the use of Impression Coping Driver **ICD00**

Description	4.1mm			5.0mm			
	Emergence Profile	5.0	6.0	7.5	5.0	6.0	7.5
Pick-Up Impression Coping	IIC12	IIC60	IIC75		WIP55	WIP56	WIP57
Twist Lock Impression Coping	IIC45	IIC46	IIC47		WIT55	WIT56	WIT57
Laboratory Analog	ILA20	ILA20	ILA20		ILAW5	ILAW5	ILAW5
Laboratory Abutment Holder	LTAH7						
Abutment Screw	UNISG*, UNIHG, UNIHT						
Square Try-In Screw (5-pack)	UNITS						
PreFormance Post	See page 47						

*Recommended

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Cement-Retained Restorations

External Hex Connection

UCLA Abutments

Indications:


- Laboratory fabricated custom abutments
- Single and multi-unit restorations
- Minimum interarch space of 6mm
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	MUCG1C
4.1mm Seating Surface	
Gold (Hexed)	GUCA1C
Gold Standard ZR™ (Hexed)	SGUCA1C
Castable (Hexed)	UNAB1C
Castable (Hexed) 25PK	UNA125
5.0mm Seating Surface	
Gold (Hexed)	WGA51C
Gold Standard ZR (Hexed)	SWGA51C
Castable (Hexed)	WPC51C
6.0mm Seating Surface	
Gold (Hexed)	WGA61C
Gold Standard ZR (Hexed)	SWGA61C
Castable (Hexed)	WPC61C




All indicated measurements are in millimeters.


Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.


Cement-Retained Restorations

External Hex Connection

UCLA Abutment Components

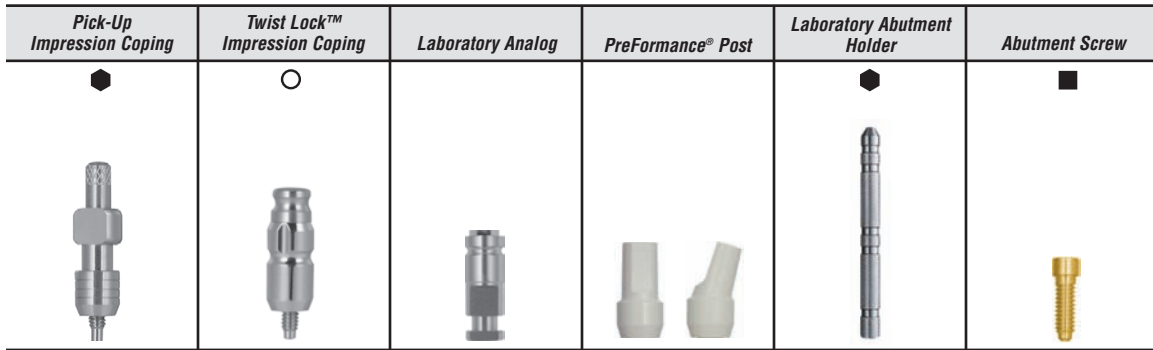

 = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

 = Requires the use of Impression Coping Driver **ICD00**

 = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

Description	3.4mm	4.1mm			5.0mm			6.0mm	
Emergence Profile	3.8	5.0	6.0	7.5	5.0	6.0	7.5	6.0	7.5
Pick-Up Impression Coping	MIC33	IIC12	IIC60	IIC75	WIP55	WIP56	WIP57	WIP66	WIP67
Twist Lock Impression Coping	N/A	IIC45	IIC46	IIC47	WIT55	WIT56	WIT57	WIT66	WIT67
Laboratory Analog	MMILA	ILA20	ILA20	ILA20	ILAW5	ILAW5	ILAW5	ILAW6	ILAW6
Laboratory Abutment Holder	LTAH5	LTAH7	LTAH7	LTAH7	LTAH7	LTAH7	LTAH7	LTAH7	LTAH7
Abutment Screw	UNISG* *, UNIHG, UNIHT								
Square Try-In Screw (5-pack)	MUNITS	UNITS							
PreFormance Post	See page 47								

* Non-Hexed
 ** Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	13.5 x 10 ⁻⁶ °K at 500°C

An alloy with a CTE of 10⁻⁶°K at 500°C is recommended.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

UCLA Abutments

Indications:


- Single and multi-unit restorations
- Minimum interarch space of 4mm
- For aesthetic restorations when tissue is limited

Material:

Machined Gold Alloy Cylinder With Plastic Unitube



Description	Item Numbers
3.4mm Seating Surface	
Gold (Hexed)	MUCG1C
Gold (Non-Hexed)	MUCG2C
Gold (Non-Hexed)	N/A
Castable (Non-Hexed)	MUCC2C
Castable (Non-Hexed)	N/A
4.1mm Seating Surface	
Gold (Hexed)	GUCA1C
Gold (Non-Hexed)	GUCA2C
Gold (Non-Hexed)	N/A
Gold Standard ZR™ (Hexed)	SGUCA1C
Castable (Hexed)	UNAB1C
Castable (Non-Hexed)	UNAB2C
Castable (Non-Hexed)	N/A
Castable (Hexed) 25PK	UNA125
Castable (Non-Hexed) 25PK	UNA225
5.0mm Seating Surface	
Gold (Hexed)	WGA51C
Gold (Non-Hexed)	WGA52C
Gold (Non-Hexed)	N/A
Gold Standard ZR (Hexed)	SWGA51C
Castable (Hexed)	WPC51C
Castable (Non-Hexed)	WPC52C
Castable (Non-Hexed)	N/A
6.0mm Seating Surface	
Gold (Hexed)	WGA61C
Gold (Non-Hexed)	WGA62C
Gold (Non-Hexed)	N/A
Gold Standard ZR (Hexed)	SWGA61C
Castable (Hexed)	WPC61C
Castable (Non-Hexed)	WPC62C
Castable (Non-Hexed)	N/A

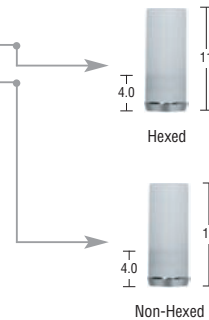


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

UCLA Abutment Cylinder Components

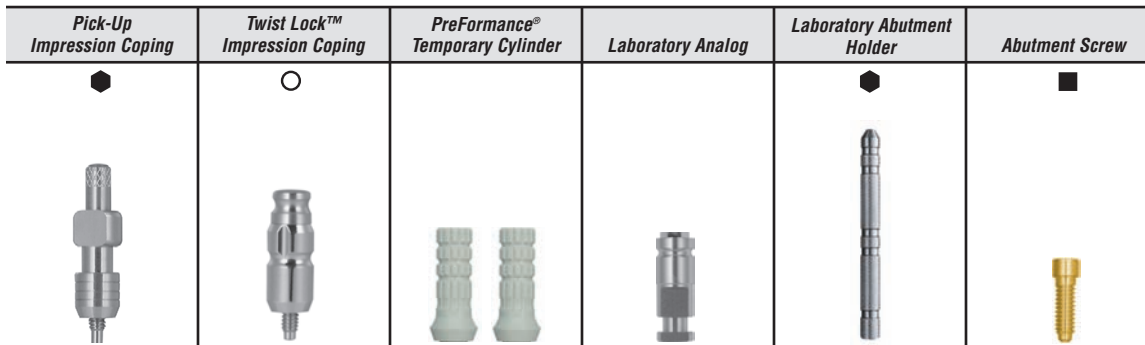

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**
○ = Requires the use of Impression Coping Driver **ICD00**
■ = Requires the use of Square Driver **PSQD0N**, **PSQD1N** or Driver Tip **RASQ3N**, **RASQ8N**

Description	3.4mm		4.1mm			5.0mm			6.0mm	
	3.8	5.0	6.0	7.5	5.0	6.0	7.5	6.0	7.5	
Pick-Up Impression Coping	MIC33	IIC12	IIC60	IIC75	WIP55	WIP56	WIP57	WIP66	WIP67	
Twist Lock Impression Coping	N/A	IIC45	IIC46	IIC47	WIT55	WIT56	WIT57	WIT66	WIT67	
Laboratory Analog	MMILA		ILA20			ILAW5		ILAW6		
Laboratory Holder	LTAH5		LTAH7			LTAH7		LTAH7		
PreFormance Temp. Cylinder	hexed ↓	MPFTC34		PFTC41		WPFTC51		WPFTC61		
	non-hexed ↓	MPFTC32		PFTC42		WPFTC52		WPFTC62		
Temporary Cylinder	hexed ↓	MMTCS1		ITCS41		WTCS51		WTCS61		
	non-hexed ↓	N/A		ITCS42		WTCS52		WTCS62		
Abutment Screw	UNISG*, UNIHG, UNIHT									
Square Try-In Screw (5-pack)	MUNITS	UNITS								

*Recommended

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Low Profile Abutments

Indications:

- Single and multi-unit screw-retained restorations
- Minimum interarch space of 7.5mm
- Minimum tissue height of 1.0mm
- Angle correction up to 30°
- External hex connection 3.4mm(D) Low Profile Abutments are limited to use in the anterior

Material:

Titanium Alloy



3.4mm Seating Surface		Item Numbers			
Collar Height	<i>Straight (One Piece)</i>	<i>Straight (Two Piece)</i>	<i>17° Pre-Angled</i>	<i>30° Pre-Angled</i>	
1.0mm	LPC341U	LPC341	N/A	N/A	
2.0mm	LPC342U	LPC342	LPAC3217	N/A	
3.0mm	LPC343U	LPC343	N/A	LPAC3330	
4.0mm	LPC344U	LPC344	LPAC3417	N/A	
5.0mm	N/A	N/A	N/A	LPAC3530	

4.1mm Seating Surface		Item Numbers			
Collar Height	<i>Straight (One Piece)</i>	<i>Straight (Two Piece)</i>	<i>17° Pre-Angled</i>	<i>30° Pre-Angled</i>	
1.0mm	LPC441U	LPC441	N/A	N/A	
2.0mm	LPC442U	LPC442	LPAC4217	N/A	
3.0mm	LPC443U	LPC443	N/A	LPAC4330	
4.0mm	LPC444U	LPC444	LPAC4417	N/A	
5.0mm	N/A	N/A	N/A	LPAC4530	

5.0mm Seating Surface		Item Numbers			
Collar Height	<i>Straight (One Piece)</i>	<i>Straight (Two Piece)</i>	<i>17° Pre-Angled</i>	<i>30° Pre-Angled</i>	
1.0mm	LPC541U	LPC541	N/A	N/A	
2.0mm	LPC542U	LPC542	LPAC5217	N/A	
3.0mm	LPC543U	LPC543	N/A	LPAC5330	
4.0mm	LPC544U	LPC544	LPAC5417	N/A	
5.0mm	N/A	N/A	N/A	LPAC5530	











All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Low Profile Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Healing Cap	Gold And Castable Cylinder
				
QuickBridge®	Temporary Cylinder	Polishing Protector	Retaining Screw	Driver And Driver Tip
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

○ = Requires the use of Impression Coping Driver ICDD00

Description		4.8mm Restorative Platform
Pick-Up Impression Coping	hexed ↓ non-hexed ↓	LPCPIC1 LPCPIC2
Twist Lock Impression Coping	hexed ↓ non-hexed ↓	LPCTIC1 LPCTIC2
QuickBridge Impression Coping		LPCRIC
Laboratory Analog		LPCLA
Temporary Cylinder	hexed ↓ non-hexed ↓	LPCTC1 LPCTC2
Healing Cap		LPCHC
PreFormance Temp. Cylinder	hexed ↓ non-hexed ↓	LPCPTC1 LPCPTC2
QuickBridge		LPCQB
QuickBridge Replacement Cap		LPCQBCAP
Distal Extension		LPCDE
Gold Cylinder	hexed ↓ non-hexed ↓	LPCGC1 LPCGC2
Castable Cylinder	hexed ↓ non-hexed ↓	LPCCC1 LPCCC2
Laser Weld Cylinder		LPCTUCA
Waxing Screw		LPCWS
Retaining Screw		LPCGSH, LPCTSH
Lapping Tool		LPCAMI
Polishing Protector		LPCPP

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection


Immediate Occlusal Loading (IOL®) Abutments*


Indications:

- Multi-unit porcelain fused to metal restorations
- Minimum interarch space of 9.2mm
- Minimum tissue height of 2mm

Material:

Titanium Alloy

4.1mm Seating Surface		
Emergence Profile	Collar Height	Item Numbers
4.5mm	2.0mm	IOL20T
4.5mm	3.0mm	IOL30T
4.5mm	4.0mm	IOL40T
4.5mm	5.5mm	IOL55T
4.5mm	7.0mm	IOL70T



Uses **PAD00** (17mm), **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip

*Indications: For surgical placement in the upper or lower jaw to provide a means for prosthetic attachment in single tooth restorations and in partially or fully edentulous spans with multiple single teeth, or as a terminal or intermediary abutment for fixed or removable bridgework and to retain overdentures.

In addition, when a minimum of 4 implants, ≥ 10mm in length, are placed in the mandible and splinted in the anterior region, immediate loading is indicated.

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

IOL® Abutment Components

<i>Pick-Up Impression Coping</i>	<i>Twist Lock™ Impression Coping</i>	<i>Laboratory Analog</i>	<i>Temporary Cylinder</i>	<i>Gold Cylinder</i>
<i>Healing Cap</i>	<i>Polishing Protector</i>	<i>Driver And Driver Tip</i>	<i>Retaining And Waxing Screw</i>	
				= Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

Description	4.1mm
Emergence Profile	4.5
Pick-Up Impression Coping	IOLPIC
Twist Lock Impression Coping	IOLTIC
Laboratory Analog	IOLLAS
Temporary Cylinder	IOLTIC
Gold Cylinder	IOLGC
Healing Cap	IOLHC
Polishing Protector	IOLPP
Driver	PAD00, PAD24
Driver Tip	RASA3
Retaining Screw	GSH30, GSH70
Waxing Screw	WSK10, WSK15

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Conical Abutments

Indications:

- Single and multi-unit porcelain fused to metal restorations
- Minimum interarch space of 9.2mm
- Minimum tissue height of 2mm

Material:

- Angled (Titanium Alloy)
- Straight (Commercially Pure Titanium)



3.4mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
3.4mm	1.0mm	MCA31	N/A	N/A
3.4mm	2.0mm	MCA32	N/A	N/A
3.4mm	3.0mm	MCA33	N/A	N/A
3.4mm	4.0mm	MCA34	N/A	N/A

4.1mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
5.0mm	1.0mm	SCA001	N/A	N/A
5.0mm	2.0mm	SCA002	AC4217	AC4225
5.0mm	3.0mm	SCA003	N/A	N/A
5.0mm	4.0mm	SCA004	AC4417	AC4425
5.0mm	5.5mm	SCA055	N/A	N/A

5.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
5.0mm	1.0mm	SWCA51	N/A	N/A
5.0mm	2.0mm	SWCA52	N/A	N/A
5.0mm	3.0mm	SWCA53	N/A	N/A
5.0mm	4.0mm	SWCA54	N/A	N/A
5.0mm	5.5mm	SWCA55	N/A	N/A

6.0mm Seating Surface

Emergence Profile	Collar Height	Item Numbers (Straight)	Item Numbers (17° Pre-Angled)	Item Numbers (25° Pre-Angled)
6.0mm	1.0mm	SWCA61*	N/A	N/A
6.0mm	2.0mm	SWCA62	N/A	N/A
6.0mm	3.0mm	SWCA63	N/A	N/A
6.0mm	4.0mm	SWCA64	N/A	N/A
6.0mm	5.5mm	SWCA65	N/A	N/A

Uses **PAD00** (17mm) or **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip.











*Requires use of GSH20 Retaining Screw.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screw-Retained Restorations

External Hex Connection

Conical Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Healing Cap	Gold And Castable Cylinder
				
QuickBridge®	Temporary Cylinder	Polishing Protector	Retaining Screw	Driver And Driver Tip
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N
 ○ = Requires the use of Impression Coping Driver ICD00

Description	3.4mm	4.1mm			5.0mm			6.0mm	
	3.8	5.0	6.0	7.5	5.0	6.0	7.5	6.0	7.5
Pick-Up Impression Coping	single-unit ↓ MEC33	CNRIC	CSQN6	CSQN7	CNRIC	CSQN6	CSQN7	WCP661	WCP671
	multi-unit ↓ N/A	CSQI7	CSQ06	CSQ07	CSQ17	CSQ06	CSQ07	WCP662	N/A
Twist Lock Impression Coping	single-unit ↓ N/A	N/A	N/A	N/A	N/A	N/A	N/A	WCT661	WCT671
	multi-unit ↓ N/A	CIC55	CIC56	CIC57	CIC55	CIC56	CIC57	WCT662	WCT672
Laboratory Analog	MMCLA	CLA20	CLA20	CLA20	CLA20	CLA20	CLA20	WCLA6	WCLA6
Healing Cap	MHC33	CS250	CS260	CS270	CS250	CS260	CS270	WCS66	WCS67
Gold Cylinder	single-unit ↓ MCAG1*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG5*	CNRG6*	CNRG6*
	multi-unit ↓ MCAG2*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC5*	CAGC6*	CAGC6*
Castable Cylinder	single-unit ↓ N/A	CNRC5*	CNRC5*	CNRC5*	CNRC5*	CNRC5*	CNRC5*	N/A	N/A
	multi-unit ↓ N/A	CACC5*	CACC5*	CACC5*	CACC5*	CACC5*	CACC5*	N/A	N/A
Temporary Cylinder	single-unit ↓ MCTC1*	CNC30*	CNC30*	CNC30*	CNC30*	CNC30*	CNC30*	WCTC60*	N/A
	multi-unit ↓ MCTC2*	CC300*	CC300*	CC300*	CC300*	CC300*	CC300*	WCTC61*	WCTC671*
QuickBridge	multi-unit ↓ N/A	QKBRG	QKBRG	QKBRG	QKBRG	QKBRG	QKBRG	N/A	N/A
Polishing Protector	PPMC1	PPCA3	PPCA3	PPCA3	PPCA3	PPCA3	PPCA3	WCPP6	WCPP6
Retaining Screw		GSH30, GSH70**						GSH20, GSH30, GSH70**	

*Requires Gold-Tite® Retaining Screw
 **Height of screw may be adjusted to access hole depth.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

Immediate Occlusal Loading (IOL®) Abutments

Indications:

- Multiple implant bar retained and fixed removable overdentures
- Minimum interarch space of 6.5mm
- Maximum angulation of 30°


Material:

Titanium Alloy

Immediate Occlusal Loading:

- Adequate bone quality equal to or greater than Type III
- Bone height equal to or greater than 12mm to allow for a minimum 10mm implant
- Bone width equal to or greater than 6mm to allow for a minimum 4mm diameter implant
- Adequate curvature of the arch and space between mental foramina, to permit proper anterior/posterior spread measurement, will allow functional cantilevers to 1st molar occlusion

4.1mm Seating Surface		Item Numbers
Emergence Profile	Collar Height	
4.5mm	2.0mm	IOL20T
4.5mm	3.0mm	IOL30T
4.5mm	4.0mm	IOL40T
4.5mm	5.5mm	IOL55T
4.5mm	7.0mm	IOL70T



Uses **PAD00** (17mm), **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

IOL® Abutment Components

<i>Pick-Up Impression Coping</i>	<i>Twist Lock™ Impression Coping</i>	<i>Laboratory Analog</i>	<i>Temporary Cylinder</i>	<i>Gold Cylinder</i>
<i>Distal Extension</i>	<i>Healing Cap</i>	<i>Polishing Protector</i>	<i>Driver And Driver Tip</i>	<i>Retaining And Waxing Screw</i>

◆ = Requires the use of Hex Driver **PHD02N**, **PHD03N** or Driver Tip **RASH3N**, **RASH8N**

Description	4.1mm
Emergence Profile	4.5
Pick-Up Impression Coping	IOLPIC
Twist Lock Impression Coping	IOLTIC
Laboratory Analog	IOLLAS
Temporary Cylinder	IOLTC
Gold Cylinder	IOLGC
Distal Extension	IOLDE
Healing Cap	IOLHC
Polishing Protector	IOLPP
Driver	PAD00, PAD24
Driver Tip	RASA3
Retaining Screw	GSH30, GSH70
Waxing Screw	WSK10, WSK15

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection



Standard Abutments

Indications:

- Multiple implant bar retained and fixed removable overdentures
- Minimum interarch space of 6.5mm
- Maximum divergence of 30°

Material:



Commercially Pure Titanium

4.1mm Seating Surface		
Collar Height	Item Numbers	
2.0mm	AB200*	
3.0mm	AB300	
4.0mm	AB400	
5.5mm	AB550	
7.0mm	AB700	
5.0mm Seating Surface		
Collar Height	Item Numbers	
2.0mm	WAB200*	
3.0mm	WAB300	
4.0mm	WAB400	
5.5mm	WAB550	



Uses **PAD00** (17mm) or **PAD24** (24mm) Abutment Driver or **RASA3** Driver Tip.

*Requires Gold-Tite® Retaining Screw (GSH20)











Temporary Healing Retention Cylinder	
Retains denture with soft tissue liner.	
	
THRC4 4.1mm(D) x 4mm(H)	THRC6 4.1mm(D) x 6mm(H)

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

Standard Abutment Components

Pick-Up Impression Coping	Twist Lock™ Impression Coping	Laboratory Analog	Gold Cylinder	Temporary Cylinder
				
Polishing Protector	Healing Cap	Retaining Screw	Driver And Driver Tip	LOCATOR® Bar Attachment
				

◆ = Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N

○ = Requires the use of Impression Coping Driver ICD00

Description	4.1mm	5.0mm
	4.5	5.5
Pick-Up Impression Coping	SQIC7	SQIC7
Twist Lock Impression Coping	SIC70	SIC70
Laboratory Analog	SLA20	SLA20
Gold Cylinder	SGC30**	SGC30**
Chamfered Gold Cylinder	CGC30**	CGC30**
Castable Plastic Cylinder	SGC34**	SGC34**
LOCATOR Bar Attachment	LOAB*	LOAB*
LOCATOR Bar Attachment Tap	LOAT	LOAT
LOCATOR Drill	LOAD	LOAD
Gold Hader Clip	ORCG1	ORCG1
Plastic Hader Clip	ORCY1	ORCY1
Temporary Cylinder	TC300**	TC300**
Polishing Protector	PPSA3	PPSA3
Healing Cap	TS250	TS250
Retaining Screw	GSH20, GSH30, GSH70***	GSH20, GSH30, GSH70***

*Includes LOCATOR Attachment, Housing, Processing Male, Spacer Males, 3 Retention Replacement Males

**Requires Gold-Tite® Retaining Screw (GSH30, GSH70).

***Height of screw may be adjusted to access hole depth.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection


LOCATOR® Abutments


Indications:


- Tissue supported removable overdentures on 2 to 4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants


Material:

Abutment: Titanium Alloy With Titanium Nitride Coating
 Housing: Titanium Alloy
 Males: Nylon



3.4mm Seating Surface		
Collar Height		Item Numbers
1.0mm		MLOA001
2.0mm		MLOA002
3.0mm		MLOA003
4.0mm		MLOA004
5.0mm		MLOA005
6.0mm		MLOA006



4.1mm Seating Surface		
Collar Height		Item Numbers
1.0mm		LOA001
2.0mm		LOA002
3.0mm		LOA003
4.0mm		LOA004
5.0mm		LOA005
6.0mm		LOA006



Included With Each Abutment:

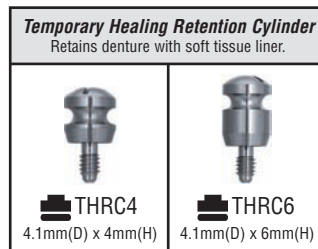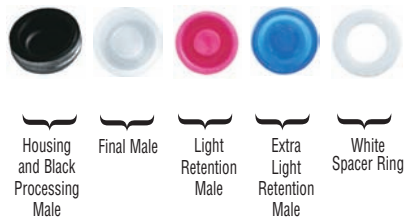





All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

LOCATOR® Abutment Components

Impression Coping	Laboratory Analog	Retention Males	Core Tool / Driver And Driver Tip
			

Description	Item Numbers
Impression Coping	LAIC1
Laboratory Analog	LALA1
Extra Light Retention Males (4-pack) - Blue, 1.5lbs/680g	LAELM
Extended Range Males (4-pack) - Green, 4lbs/1800g	LAERM
Extra Light Retention Extended Range Males - Red, 1.5lbs/680g	LELARM
Replacement Males (4-pack) - White, 5lbs/2250g	LARMS
Light Retention Replacement Males (4-pack) - Pink, 3lbs/1350g	LLRMS
Replacement Housing	LOAH
Replacement Housing Kit	LORHK*
Core Tool/Abutment Driver	LCTDR1
Driver Tip 24mm(L)	LOADT4
Driver Tip 30mm(L)	LOADT9
1.25mm/.050in. Driver Tip 24mm(L) - used with LCTDR1	RASH4
1.25mm/.050in. Driver Tip 30mm(L) - used with LCTDR1	RASH9
LOCATOR Bar Attachment	LOAB
LOCATOR Bar Attachment Tap	LOAT
LOCATOR Bar Attachment Drill	LOAD

*Included With **LORHK**
Replacement Housing Kit:



External Hex Connection

Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection


O-Ring Abutments

Indications:

- Tissue supported overdenture retained by 2 or more implants
- Partial overdentures
- Resilient retention
- Minimum interarch space of 7mm
- Maximum tissue height of 6mm
- Recommended for parallel implants; (see castable O-Ring system for divergent implants)
- 850 grams of retention



Material:

Abutment: Commercially Pure Titanium
 O-Ring: Buna
 Housing: Titanium Alloy

4.1mm Seating Surface		
Collar Height	Item Numbers	
2.0mm	OSO20	
4.0mm	OSO40	
6.0mm	OSO60	
5.0mm Seating Surface		
Collar Height	Item Numbers	
2.0mm	WOSO20	
4.0mm	WOSO40	
6.0mm	WOSO60	



Included With Each Abutment:

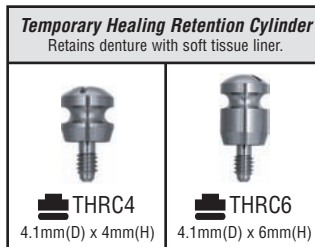





All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

O-Ring Abutment Components

Laboratory Analog	Housing	O-Ring	Driver And Driver Tip
			

Description	Item Numbers
Laboratory Analog	ORLAU
Housing	OSODH
O-Ring Replacement	OSOBLK
Red Processing O-Ring	OSORED
O-Ring/Dal-Ro Abutment Driver	PAD01
O-Ring/Dal-Ro Abutment Driver Tip	RAOR1
Castable System	OSOCA*

*Use with UCLA Abutment to realign non-parallel implants or on distal of overdenture bar.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection


Dal-Ro Abutments


Indications:

- Tissue supported overdentures
- Partial overdentures
- Rigid retention
- Minimum interarch space of 5mm
- Maximum tissue height of 6mm
- Recommended for parallel implants; (see castable Dal-Ro system for divergent implants)
- 250–1000 grams of retention; may be adjusted



Material:

Abutment: Titanium Alloy
 Housing: Titanium
 Females: Gold Alloy

4.1mm Seating Surface		
Emergence Profile		Item Numbers
2.0mm		DRH20
4.0mm		DRH40
6.0mm		DRH60



Included With Each Abutment:

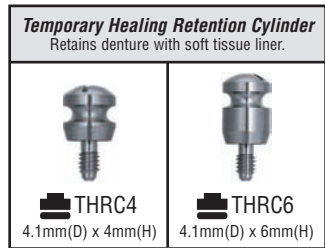






All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

OverdentSURE Restorations

External Hex Connection

Dal-Ro Abutment Components

Laboratory Analog	Housing/Female Assembly	Replacement Female	Female Adjustment Tool	Driver And Driver Tip
				

Description	Item Numbers
Laboratory Analog	DRLAU
Housing/Female Assembly	DRTH
Replacement Female	DRAF
Female Adjustment Tool	DRFAT1
O-Ring/Dal-Ro Abutment Driver	PAD01
O-Ring/Dal-Ro Abutment Driver Tip	RAOR1
Castable System	DRCS1*

*Use with UCLA Abutment to realign non-parallel implants or on distal of hader bar.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

External Hex Connection


PreFormance® Posts

Indications:

- Single and multiple unit provisional cement-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft tissue healing of single and multiple unit restorations of integrated implants

Material:

PEEK: Titanium Alloy Connection

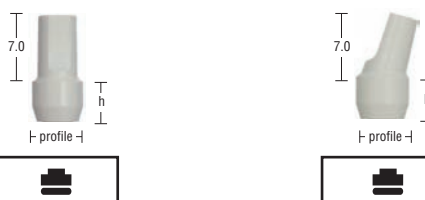

3.4mm Seating Surface			
<i>Emergence Profile</i>	<i>Collar Height</i>	<i>Item Numbers (Straight)</i>	<i>Item Numbers (15° Pre-Angled)</i>
3.8mm	4.0mm	MPFP34	MPAPF34
3.8mm	6.0mm	MPFP36	MPAPF36
4.1mm Seating Surface			
<i>Emergence Profile</i>	<i>Collar Height</i>	<i>Item Numbers (Straight)</i>	<i>Item Numbers (15° Pre-Angled)</i>
5.0mm	4.0mm	PFP454	PAPF454
5.0mm	6.0mm	PFP456	PAPF456
5.0mm Seating Surface			
<i>Emergence Profile</i>	<i>Collar Height</i>	<i>Item Numbers (Straight)</i>	<i>Item Numbers (15° Pre-Angled)</i>
5.0mm	4.0mm	WPFP554	PAPF554
5.0mm	6.0mm	WPFP556	PAPF556
6.0mm Seating Surface			
<i>Emergence Profile</i>	<i>Collar Height</i>	<i>Item Numbers (Straight)</i>	<i>Item Numbers (15° Pre-Angled)</i>
6.0mm	4.0mm	WPFP664	PAPF664
6.0mm	6.0mm	WPFP666	PAPF666

All PreFormance Posts are packaged with a Titanium Hexed Screw (UNIHT).

All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Provisional Restorations

External Hex Connection

PreFormance® Temporary Cylinders

Indications:


- Single and multiple unit provisional screw-retained restorations
- Minimum interarch space of 6mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single and multiple unit restorations of integrated implants for guided tissue healing

Material:

PEEK: Titanium Alloy Connection



Description	Item Numbers
3.4mm Seating Surface	
Hexed	MPFTC34
Non-Hexed	MPFTC32
4.1mm Seating Surface	
Hexed	PFTC41
Non-Hexed	PFTC42
5.0mm Seating Surface	
Hexed	WPFTC51
Non-Hexed	WPFTC52
6.0mm Seating Surface	
Hexed	WPFTC61
Non-Hexed	WPFTC62



All PreFormance Cylinders are packaged with a Titanium Hexed Screw (UNIHT).


All indicated measurements are in millimeters.

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screws


Certain® Internal Connection

Abutment Screws




	Gold-Tite® Screw	Titanium Screw	Large Gold-Tite Screw	Large Titanium Screw
Screws	IUNIHG, IZSHG	IUNIHT	ILRGHG	ILRGHT
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	20Ncm	20Ncm	20Ncm	20Ncm
For Use With:	UCLA Abutment, GingiHue® Post, GingiHue Post 15°, IZSHG - ZiReal® Post, Hexed Temporary Cylinder, Provide®		Non-Hexed UCLA Abutment, Non-Hexed Temporary Cylinder, CAM StructSURE® Precision Milled Bars	

Waxing Screws And Try-In Screws



	Laboratory Screw	Hex (5-pack) Try-In Screw
Screws	IWSU30	IUNITS
Drivers	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N
For Use With:	Pick-Up and Impression Copings, Implant Level Laboratory Procedures	Hexed UCLA Abutment, GingiHue Post, GingiHue Post 15°, Provide Abutment

Retaining Screws



	Gold-Tite Retaining Screw
Screws	GSH20, GSH30, GSH70
Drivers	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N
Torque	10Ncm
For Use With:	GSH20 - Standard Abutment 6mm(D) X 2mm(H) Conical Abutment 6mm(D) X 1mm(H) GSH30 - Standard, Conical and IOL® Abutments GSH70 - Standard, Conical and IOL Abutments

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Screws

External Hex Connection

Abutment Screws And Retaining Screws



	Gold-Tite® Square Abutment Screw	Gold-Tite Hexed Abutment Screw	Titanium Hexed Abutment Screw	Gold-Tite Retaining Screw
Screws	UNISG	UNIHG	UNIHT	GSH20, GSH30, GSH70
Drivers	PSQD0N, PSQD1N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASQ3N, RASQ8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	32–35Ncm	20Ncm	20Ncm	10Ncm
For Use With:	UCLA Abutment, GingiHue® Post, GingiHue Post 15°, ZiReal® Post, Titanium Cylinder			GSH20 - Standard Abutment 6mm(D) X 2mm(H) Conical Abutment 6mm(D) X 1mm(H) GSH30 - Standard, Conical and IOL® Abutments GSH70 - Standard, Conical and IOL Abutments

Waxing Screws And Try-In Screws




	Abutment Waxing Screw/Guide Pin	Laboratory Waxing Screw	Square Try-In Screw (5-pack)
Screws	WSK10, WSK15, WSK30	WSU30	UNITS, MUNITS
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PSQD0N, PSQD1N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASQ3N, RASQ8N
For Use With:	Standard and Conical Abutments	Implant Level Laboratory Procedures	UCLA Abutment, GingiHue Post, GingiHue Post 15°, ZiReal Post


Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Mechanical Driver Kits

NCATDO Contra Angle Torque Driver Kit

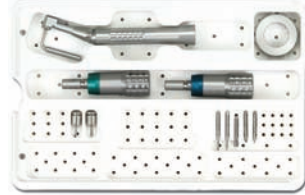

NPSDKO Prosthetic Driver Kit

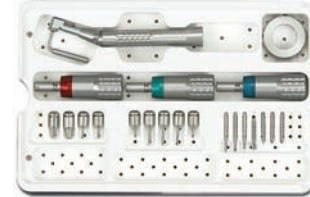

NCATDOC Contra Angle Torque Driver Kit Certain®




L-TIRW Low Torque Indicating Ratchet Wrench






NCATDO Contra Angle Torque Kit	NCATDOC Contra Angle Torque Kit Certain	NPSDKO Prosthetic Driver Kit	L-TIRW Low Torque Indicating Kit	Description	Item Numbers
•	•	•		Narrow Posterior Hex Driver, 17mm(L)	PHD02N
•		•		Narrow Posterior Square Driver, 17mm(L)	PSQD0N
•	•	•		Contra Angle Torque Driver Body	HTD-C
•	•	•	•	Narrow Right Angle Hex Driver Tip, 24mm(L)	RASH3N
•	•	•		Narrow Right Angle Hex Driver Tip, 30mm(L)	RASH8N
•		•	•	Narrow Right Angle Square Driver Tip, 24mm(L)	RASQ3N
•		•		Narrow Right Angle Square Driver Tip, 30mm(L)	RASQ8N
•	•	•		Right Angle Abutment Driver Tip - Steel	RASA3
		•		Contra Angle Torque Controller, 10Ncm	TD-10
•	•	•		Contra Angle Torque Controller, 20Ncm	TD-20
•		•		Contra Angle Torque Controller, 35Ncm	TD-35
•	•	•		Contra Pre-action Handle	CATDH
•	•	•		Prosthetic System Driver Tray	PSDT1
		•		Narrow Impression Coping Driver	ICD00
		•		Posterior Abutment Driver, 17mm(L)	PAD00
		•		Standard Abutment Driver, 24mm(L)	PAD24
		•		Posterior Slotted Screw Driver, 17mm(L)	PSD00
		•		Standard Slotted Screw Driver, 24mm(L)	PSD01
		•		Narrow Standard Slotted Square Driver, 24mm(L)	PSQD1N
		•		Narrow Standard Hex Driver, 24mm(L)	PHD03N
		•		Right Angle Slotted Driver Tip, 24mm(L)	RASD1
		•		Right Angle Slotted Driver Tip, 30mm(L)	RASD6
			•	Low Torque Indicating Ratchet Wrench	L-TIRW
			•	Restorative Torque Tray	RTI2035TR

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Drivers And Driver Tips


							
		Small Hex		Large Hex		Square	
Length	Driver	Tip	Driver	Tip	Driver	Tip	
17mm	PHD00N	N/A	PHD02N	N/A	PSQD0N	N/A	
24mm	PHD01N	RASH2N	PHD03N	RASH3N	PSQD1N	RASQ3N	
30mm	N/A	RASH7N	N/A	RASH8N	N/A	RASQ8N	
For Use With:	External Hex Cover Screws		Healing Abutments, Abutment Screws, Certain® Cover Screws and Retaining Screws		Square Gold-Tite® Abutment Screws and Square Try-in Screws		

						
		O-Ring/Dal-Ro		Abutment		LOCATOR®
Length	Driver	Tip	Driver	Tip	Tip Only	
17mm	N/A	N/A	PAD00	N/A	N/A	
24mm	PAD01	RAOR1	PAD24	RASA3	LOADT4	
30mm	N/A	N/A	N/A	N/A	LOADT9	
For Use With:	O-Ring Abutments and Dal-Ro Abutments		Low Profile, Conical Abutments, Standard Abutments and IOL® Abutments		LOCATOR Abutments	

			<div style="background-color: #333; color: white; padding: 5px; font-weight: bold; text-align: left;">MIDTH</div> <div style="text-align: left; padding: 5px;">Manual Interchangeable Driver Tip Handle</div> 	
		Impression Coping		.050" Hex
Length	Driver Only	Tip Only		
17mm	ICD00	N/A		
24mm	N/A	RASH4		
30mm	N/A	RASH9		
For Use With:	Twist Lock™ Transfer Impression Copings	LOCATOR Abutments with LOCATOR Core Tools		

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Navigator® System Instrumentation Overview

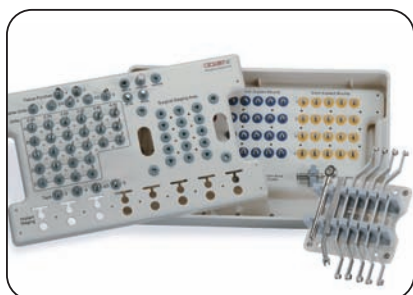

Navigator Surgical Kit



Navigator Laboratory Kit

The Navigator System For CT Guided Surgery

The Navigator System offers the instrumentation that clinicians need to transform computer-based planning into practical implant placement with an opportunity for immediate provisionalization.

The Navigator System features control of hex-orientation to fabricate and deliver provisional restorations for BIOMET 3i Parallel Walled Certain® 3.4, 4.1 and 5mm Implant Platforms, immediately following surgery. This unique hex-orientation feature is especially beneficial when immediately loading single tooth cases, cement-retained cases and cases where angulation correction is required.

An integral part of the Navigator System is the Navigator Laboratory Kit, which contains easy-to-identify components needed to fabricate a master cast and provisional prosthesis prior to the day of surgery.


The Navigator Laboratory Kit provides you with the opportunity to:

- Treat Patients For Immediate-Load Cases
- Be Part Of A Collaborative Approach To Comprehensive Patient Treatment
- Embrace Emerging Technology

Navigator® Laboratory Kit

SGLKIT Navigator Laboratory Kit




		
SGLKIT Laboratory Kit	Description	Item Numbers
•	Navigator Laboratory Tray	SGLTRAY
•	Navigator Certain® Analog Mount, 3.4mm(D) x 1(L)	MSGIAM1
•	Navigator Certain Analog Mount, 3.4mm(D) x 2(L)	MSGIAM2
•	Navigator Certain Analog Mount, 3.4mm(D) x 3(L)	MSGIAM3
•	Navigator Certain Analog Mount, 3.4mm(D) x 4(L)	MSGIAM4
•	Navigator Certain Analog Mount, 4.1mm(D) x 1(L)	SGIAM41
•	Navigator Certain Analog Mount, 4.1mm(D) x 2(L)	SGIAM42
•	Navigator Certain Analog Mount, 4.1mm(D) x 3(L)	SGIAM43
•	Navigator Certain Analog Mount, 4.1mm(D) x 4(L)	SGIAM44
•	Navigator Certain Analog Mount, 5mm(D) x 1(L)	SGIAM51
•	Navigator Certain Analog Mount, 5mm(D) x 2(L)	SGIAM52
•	Navigator Certain Analog Mount, 5mm(D) x 3(L)	SGIAM53
•	Navigator Certain Analog Mount, 5mm(D) x 4(L)	SGIAM54

Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Laboratory Tools

Lapping Tool For Castable UCLA Abutment With Guide

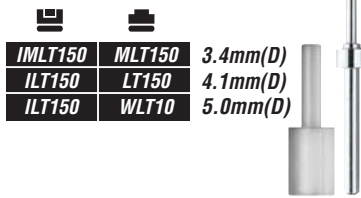

RH600 Reamer With Handle




PPMC1 Polishing Protector, 3.4mm(D) Conical Abutment

PPCA3
4.1mm(D)
5.0mm(D)


WCPP6
6.0mm(D)



Polishing Protector, UCLA Abutment

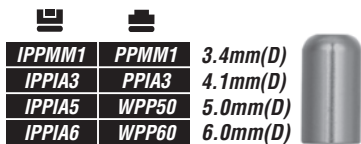

Laboratory Abutment Holder

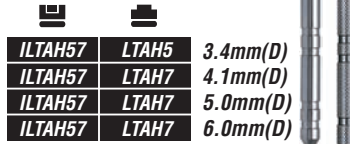

PPSA3 Polishing Protector, 4.1mm(D) Standard Abutment




IQSA01 **Certain® QuickSeat® Activator Tool**



Miscellaneous Items


TMP80 Tissue Measuring Post



SRT10 Screw Removal Kit



AG900 Prosthetic Angle Guide Kit



ISRT10 Certain Screw Removal Kit



Some products may not be available outside of the United States.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

Professional Development Products

Tools For The Art Of Business Building



BIOMET **3i** has a dedicated Professional Development Team and a comprehensive Practice Enhancement Portfolio. This portfolio includes tools for marketing, professional education and patient awareness education. Current available materials include (but are not limited to) the following:

Description	Item Numbers
BIOMET 3i IDS™ “Creating & Driving Your Own Study Club” Guidebook	ART895
3x Model of GingiHue® Post 4mm(D) x 5mm(D) x 2mm(H) with Square Screw	APPGMOD1
3x Model of OSSEOTITE® Implant 4mm(D) x 13mm(L)	OSSMOD1
3x Model of OSSEOTITE Tapered Implant	NTMOD1
3x Model Set with OSSEOTITE Tapered Certain® Implant & GingiHue Post	INTMODSET
Patient Care Card (25pk)	ART930
Patient Ed Flip Chart (electronic version only)	ART943
Patient Ed Folio with DVD (electronic version only)	ART884
Patient Ed Brochure - Bone Loss (25pk)	ART885
Patient Ed Brochure - Single Tooth (25pk) (electronic version only)	ART886
Patient Ed Brochure - Multiple Teeth (25pk)	ART887
Patient Ed Brochure - Implant Retained, Bar (25pk)	ART890
Patient Ed Brochure - Implant Retained, Fixed (25pk)	ART888
Patient Ed Brochure - Implant Retained, LOCATOR® (25pk)	ART889
Patient Ed Brochure - Immediate Teeth Replacement, DIEM® (25pk)	ART929
Patient Ed Brochure - Spanish Version (Bone Loss)	ART957S
Patient Ed Brochure - Spanish Version (electronic version only)	ART958S
Patient Ed DVD - Multilingual Version	ART951EUR
Patient Ed Model - LOCATOR	PEMODLOC
Patient Ed Model - Single/Multiple Teeth	PEMODSM
Patient Ed Poster	ART962
Wrench for Tightening Model Screws	MODWRENCH



Some products may not be available outside of the United States.
 Algunos productos no se comercializan fuera de EE.UU.
 Certains produits ne sont pas disponibles en dehors des États-Unis.
 Einige Produkte sind außerhalb der USA nicht erhältlich.

Index

Cat.#	Description	Page#	Cat.#	Description	Page#
AB200	STANDARD ABUTMENT 4.1MM(D) X 2MM(H)	43	DRCS1	DAL-RO CASTABLE SYSTEM	50
AB300	STANDARD ABUTMENT 4.1MM(D) X 3MM(H)	43	DRFAT1	DAL-RO FEMALE ATTACHMENT TOOL	50
AB400	STANDARD ABUTMENT 4.1MM(D) X 4MM(H)	43	DRH20	DAL-RO ABUTMENT 4.1MM(D) X 2MM(H)	49
AB550	STANDARD ABUTMENT 4.1MM(D) X 5.5MM(H)	43	DRH40	DAL-RO ABUTMENT 4.1MM(D) X 4MM(H)	49
AB700	STANDARD ABUTMENT 4.1MM(D) X 7MM(H)	43	DRH60	DAL-RO ABUTMENT 4.1MM(D) X 6MM(H)	49
AC4217	PRE-ANGLED 17° CONICAL ABUTMENT 4.1MM(D) X 2MM(H)	39	DRLAU	DAL-RO UNIVERSAL LABORATORY ANALOG	50
AC4225	PRE-ANGLED 25° CONICAL ABUTMENT 4.1MM(D) X 2MM(H)	39	DRTH	DAL-RO HOUSING/FEMALE ASSEMBLY	50
AC4417	PRE-ANGLED 17° CONICAL ABUTMENT 4.1MM(D) X 4MM(H)	39	GSH20	GOLD-TITE® (HEXED) RETAINING SCREW 2MM	18,22,40,44,53,54
AC4425	PRE-ANGLED 25° CONICAL ABUTMENT 4.1MM(D) X 4MM(H)	39	GSH30	GOLD-TITE (HEXED) RETAINING SCREW 3MM	16,18,20,22,38,40,42,44,53,54
AG900	PROSTHETIC ANGLE GUIDE KIT (9PC SET)	59	GSH70	GOLD-TITE (HEXED) RETAINING SCREW 7MM	16,18,20,22,38,40,42,44,53,54
APP452G	GINGIHUE® POST 4.1MM(D) X 5MM(P) X 2MM(H)	27	GUCA1C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 4.1MM(D)	31,33
APP454G	GINGIHUE POST 4.1MM(D) X 5MM(P) X 4MM(H)	27	GUCA2C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 4.1MM(D)	33
APP462G	GINGIHUE POST 4.1MM(D) X 6MM(P) X 2MM(H)	27	HTD-C	CONTRA ANGLE TORQUE DRIVER BODY	55
APP464G	GINGIHUE POST 4.1MM(D) X 6MM(P) X 4MM(H)	27	IAB200	CERTAIN® STANDARD ABUTMENT 4.1MM(D) X 2MM(H)	21
APP472G	GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	27	IAB300	CERTAIN STANDARD ABUTMENT 4.1MM(D) X 3MM(H)	21
APP474G	GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	27	IAB400	CERTAIN STANDARD ABUTMENT 4.1MM(D) X 4MM(H)	21
APPGMOD1	3X MODEL OF GINGIHUE POST 4MM(D) X 5MM(D) X 2MM(H) WITH SQUARE SCREW	60	IAB550	CERTAIN STANDARD ABUTMENT 4.1MM(D) X 5.5MM(H)	21
			IAB700	CERTAIN STANDARD ABUTMENT 4.1MM(D) X 7MM(H)	21
ART884	PATIENT ED FOLIO WITH DVD (ELECTRONIC VERSION ONLY)	60	IAC4217	CERTAIN PRE-ANGLED 17° CONICAL ABUTMENT 4.1MM(D) X 2MM(H)	17
ART885	PATIENT ED BROCHURE - BONE LOSS (25PK)	60	IAC4225	CERTAIN PRE-ANGLED 25° CONICAL ABUTMENT 4.1MM(D) X 2MM(H)	17
ART886	PATIENT ED BROCHURE - SINGLE TOOTH (25PK) (ELECTRONIC VERSION)	60	IAC4417	CERTAIN PRE-ANGLED 17° CONICAL ABUTMENT 4.1MM(D) X 4MM(H)	17
ART887	PATIENT ED BROCHURE - MULTIPLE TEETH (25PK)	60	IAC4425	CERTAIN PRE-ANGLED 25° CONICAL ABUTMENT 4.1MM(D) X 4MM(H)	17
ART888	PATIENT ED BROCHURE - IMPLANT RETAINED, FIXED (25PK)	60	IAPP452G	CERTAIN GINGIHUE POST 4.1MM(D) X 5MM(P) X 2MM(H)	5
ART889	PATIENT ED BROCHURE - IMPLANT RETAINED, LOCATOR® (25PK)	60	IAPP454G	CERTAIN GINGIHUE POST 4.1MM(D) X 5MM(P) X 4MM(H)	5
ART890	PATIENT ED BROCHURE - IMPLANT RETAINED, BAR (25PK)	60	IAPP462G	CERTAIN GINGIHUE POST 4.1MM(D) X 6MM(P) X 2MM(H)	5
ART895	BIOMET 3i IDS™ "CREATING & DRIVING YOUR OWN STUDY CLUB" GUIDEBOOK	60	IAPP464G	CERTAIN GINGIHUE POST 4.1MM(D) X 6MM(P) X 4MM(H)	5
			IAPP472G	CERTAIN GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	5
ART929	PATIENT ED BROCHURE - IMMEDIATE TEETH REPLACEMENT, DIEM® (25PK)	60	IAPP474G	CERTAIN GINGIHUE POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	5
ART930	PATIENT CARE CARD (25PK)	60	ICA001	CERTAIN CONICAL ABUTMENT 4.1MM(D) X 1MM(H)	17
ART943	PATIENT ED FLIP CHART (ELECTRONIC VERSION ONLY)	60	ICA002	CERTAIN CONICAL ABUTMENT 4.1MM(D) X 2MM(H)	17
ART951EUR	PATIENT ED DVD - MULTILINGUAL VERSION	60	ICA003	CERTAIN CONICAL ABUTMENT 4.1MM(D) X 3MM(H)	17
ART957S	PATIENT ED BROCHURE - SPANISH VERSION (BONE LOSS)	60	ICA004	CERTAIN CONICAL ABUTMENT 4.1MM(D) X 4MM(H)	17
ART958S	PATIENT ED BROCHURE - SPANISH (ELECTRONIC VERSION ONLY)	60	ICA055	CERTAIN CONICAL ABUTMENT 4.1MM(D) X 5.5MM(H)	17
ART962	PATIENT ED POSTER	60	ICAP454	CERTAIN ZIREAL POST 4.1MM(D) X 5MM(P) X 4MM(H)	7
CACC5	CONICAL CASTABLE CYLINDER (NON-HEXED) 4.1MM & 5MM(D)	18,40	ICAP464	CERTAIN ZIREAL POST 4.1MM(D) X 6MM(P) X 4MM(H)	7
CAGC5	CONICAL GOLD CYLINDER (NON-HEXED) 4.1MM & 5MM(D)	18,40	ICD00	NARROW IMPRESSION COPING DRIVER	55,56
CAGC6	CONICAL GOLD CYLINDER (NON-HEXED) 6MM(D)	18,40		3.4MM(D) X 3.8MM(P) X 3MM(H) X 4MM(D) X 8.5MM(L)	
CAP454	ZIREAL® POST 4.1MM(D) X 5MM(P) X 4MM(H)	29	IGUCA1C	CERTAIN UCLA GOLD HEXED ABUTMENT CYLINDER 4.1MM(D)	9,11
CAP464	ZIREAL POST 4.1MM(D) X 6MM(P) X 4MM(H)	29	IGUCA2C	CERTAIN UCLA GOLD NON-HEXED ABUTMENT CYLINDER 4.1MM(D)	11
CATDH	CONTRA PRE-ACTION HANDLE	55	IGUCA2T	CERTAIN UCLA GOLD NON-HEXED ABUTMENT CYLINDER 4.1MM(D)	11
CC300	CONICAL TEMPORARY CYLINDER (NON-HEXED) 4.1 & 5MM(D)	18,40	IIC12	IMPLANT EP PICK-UP COPING 4.1MM(D) X 5MM(P)	28,30,32,34
CGC30	CHAMFERED GOLD CYLINDER FOR STANDARD ABUTMENT	22,44	IIC45	IMPLANT EP TWIST LOCK COPING 4.1MM(D) X 5MM(P)	28,30,32,34
CIC55	CONICAL EP® TWIST LOCK™ COPING 4.1 & 5MM(D) X 5MM(P)	18,40	IIC46	IMPLANT EP TWIST LOCK COPING 4.1MM(D) X 6MM(P)	28,30,32,34
CIC56	CONICAL EP TWIST LOCK COPING 4.1 & 5MM(D) X 6MM(P)	18,40	IIC47	IMPLANT EP TWIST LOCK COPING 4.1MM(D) X 7.5MM(P)	28,30,32,34
CIC57	CONICAL EP TWIST LOCK COPING 4.1 & 5MM(D) X 7.5MM(P)	18,40	IIC60	IMPLANT EP PICK-UP COPING 4.1MM(D) X 6MM(P)	28,30,32,34
CLA20	CONICAL ABUTMENT LAB ANALOG 4.1 & 5MM(D)	18,40	IIC75	IMPLANT EP PICK-UP COPING 4.1MM(D) X 7.5MM(P)	28,30,32,34
CNC30	CONICAL TEMPORARY CYLINDER (HEXED) 4.1 & 5MM(D)	18,40	IIC12	CERTAIN EP PICK-UP COPING 4.1MM(D) X 5MM(P)	6,8,10,12
CNRC5	CONICAL CASTABLE CYLINDER (HEXED) 4.1MM & 5MM(D)	18,40	IIC41	CERTAIN EP PICK-UP COPING 4.1MM(D) X 4.1MM(P)	6,8,10,12
CNRG5	CONICAL GOLD CYLINDER (HEXED) 4.1 & 5MM(D)	18,40	IIC42	CERTAIN EP PICK-UP COPING (NON-HEXED) 4.1MM(D) X 4.1MM(P)	6,8,10,12
CNRG6	CONICAL GOLD CYLINDER (HEXED) 6MM(D)	18,40	IIC44	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 4.1MM(P)	6,8,10,12
CNRIC	CONICAL EP PICK-UP COPING (HEXED) 4.1 & 5MM(D) X 5MM(P)	18,40	IIC45	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 5MM(P)	6,8,10,12
CS250	CONICAL EP HEALING CAP 4.1MM & 5MM(D) X 5MM(P)	18,40	IIC46	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 6MM(P)	6,8,10,12
CS260	CONICAL EP HEALING CAP 4.1MM & 5MM(D) X 6MM(P)	18,40	IIC47	CERTAIN EP TWIST LOCK COPING 4.1MM(D) X 7.5MM(P)	6,8,10,12
CS270	CONICAL EP HEALING CAP 4.1MM & 5MM(D) X 7.5MM(P)	18,40	IIC60	CERTAIN EP PICK-UP COPING 4.1MM(D) X 6MM(P)	6,8,10,12
CSQ06	CONICAL EP PICK-UP COPING (NON-HEXED) 4.1 & 5MM(D) X 6MM(P)	18,40	IIC75	CERTAIN EP PICK-UP COPING 4.1MM(D) X 7.5MM(P)	6,8,10,12
CSQ07	CONICAL EP PICK-UP COPING (NON-HEXED) 4.1 & 5MM(D) X 7.5MM(P)	18,40	IILA20	CERTAIN IMPLANT LAB ANALOG 4.1MM(D)	6,8,10,12
			IILAW5	CERTAIN IMPLANT LAB ANALOG 5MM(D)	6,8,10,12
CSQI7	CONICAL EP PICK-UP COPING (NON-HEXED) 4.1 & 5MM(D) X 5MM(P)	18,40	IILAW6	CERTAIN IMPLANT LAB ANALOG 6MM(D)	6,10,12
CSQN6	CONICAL EP PICK-UP COPING (HEXED) 4.1 & 5MM(D) X 6MM(P)	18,40	IOL20S	CERTAIN IOL® ABUTMENT 2MM(H)	15,19
CSQN7	CONICAL EP PICK-UP COPING (HEXED) 4.1 & 5MM(D) X 7.5MM(P)	18,40	IOL30S	CERTAIN IOL ABUTMENT 3MM(H)	15,19
DRAF	DAL-RO REPLACEMENT FEMALE	50	IOL40S	CERTAIN IOL ABUTMENT 4MM(H)	15,19

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
I10L55S	CERTAIN® IOL® ABUTMENT 5.5MM(H)	15,19	IMCA34	CERTAIN CONICAL ABUTMENT 3.4MM(D) X 4MM(H)	17
I10L70S	CERTAIN IOL ABUTMENT 7MM(H)	15,19	IMIC30	CERTAIN EP® PICK-UP COPING 3.4MM(D) X 3.4MM(P)	6,10,12
IITCS41	CERTAIN TEMPORARY (HEXED) CYLINDER 4.1MM(D) W/HEXED SCREW	12	IMIC33	CERTAIN EP PICK-UP COPING 3.4MM(D) X 3.8MM(P)	6,10,12
IITCS42	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 4.1MM(D) W/LARGE DIA. SCREW	12	IMLOA001	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 1MM(H)	23
ILA20	IMPLANT LAB ANALOG 4.1MM(D)	28,30,32,34	IMLOA002	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 2MM(H)	23
ILAW5	IMPLANT LAB ANALOG 5MM(D)	28,30,32,34	IMLOA003	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 3MM(H)	23
ILAW6	IMPLANT LAB ANALOG 6MM(D)	28,32,34	IMLOA004	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 4MM(H)	23
ILOA001	CERTAIN LOCATOR® ABUTMENT 4.1MM(D) X 1MM(H)	23	IMLOA005	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 5MM(H)	23
ILOA002	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 2MM(H)	23	IMLOA006	CERTAIN LOCATOR ABUTMENT 3.4MM(D) X 6MM(H)	23
ILOA003	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 3MM(H)	23	IMLT150	CERTAIN LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE, 3.4MM(D)	59
ILOA004	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 4MM(H)	23	IMMILA	CERTAIN IMPLANT LAB ANALOG 3.4MM(D)	6,10,12
ILOA005	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 5MM(H)	23	IMMTCS1	CERTAIN TEMPORARY HEXED CYLINDER 3.4MM(D) W/HEXED SCREW	12
ILOA006	CERTAIN LOCATOR ABUTMENT 4.1MM(D) X 6MM(H)	23	IMPAP32G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	5
ILPAC3217	CERTAIN LOW PROFILE 17° ABUTMENT 3.4MM(D) X 2MM(H)	13	IMPAP34G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	5
ILPAC3330	CERTAIN LOW PROFILE 30° ABUTMENT 3.4MM(D) X 3MM(H)	13	IMPAPF34	CERTAIN PREFORMANCE® 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	25
ILPAC3417	CERTAIN LOW PROFILE 17° ABUTMENT 3.4MM(D) X 4MM(H)	13	IMPAPF36	CERTAIN PREFORMANCE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	25
ILPAC3530	CERTAIN LOW PROFILE 30° ABUTMENT 3.4MM(D) X 5MM(H)	13	IMPFP34	CERTAIN PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	25
ILPAC4217	CERTAIN LOW PROFILE 17° ABUTMENT 4.1MM(D) X 2MM(H)	13	IMPFP36	CERTAIN PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	25
ILPAC4330	CERTAIN LOW PROFILE 30° ABUTMENT 4.1MM(D) X 3MM(H)	13	IMPFTC32	CERTAIN PREFORMANCE TEMPORARY CYLINDER 3.4MM (NON-HEXED)	12,26
ILPAC4417	CERTAIN LOW PROFILE 17° ABUTMENT 4.1MM(D) X 4MM(H)	13	IMPFTC34	CERTAIN PREFORMANCE TEMPORARY CYLINDER 3.4MM (HEXED)	12,26
ILPAC4530	CERTAIN LOW PROFILE 30° ABUTMENT 4.1MM(D) X 5MM(H)	13	IMUCC2C	CERTAIN UCLA CASTABLE NON-HEXED ABUTMENT CYLINDER 3.4MM(D)11	
ILPAC5217	CERTAIN LOW PROFILE 17° ABUTMENT 5.0MM(D) X 2MM(H)	13	IMUCC2T	CERTAIN UCLA CASTABLE NON-HEXED ABUTMENT CYLINDER 3.4MM(D)11	
ILPAC5330	CERTAIN LOW PROFILE 30° ABUTMENT 5.0MM(D) X 3MM(H)	13	IMUGG1C	CERTAIN UCLA GOLD HEXED ABUTMENT CYLINDER 3.4MM(D)	9,11
ILPAC5417	CERTAIN LOW PROFILE 17° ABUTMENT 5.0MM(D) X 4MM(H)	13	IMUGG2C	CERTAIN UCLA GOLD NON-HEXED ABUTMENT CYLINDER 3.4MM(D)	11
ILPAC5530	CERTAIN LOW PROFILE 30° ABUTMENT 5.0MM(D) X 5MM(H)	13	IMUGG2T	CERTAIN UCLA GOLD NON-HEXED ABUTMENT CYLINDER 3.4MM(D) W/TI SCREW	11
ILPC341	CERTAIN LOW PROFILE ABUTMENT 3.4MM(D) X 1MM(H)	13	INTMODSET	3X MODEL SET WITH OSSEOTITE® TAPERED CERTAIN IMPLANT AND GINGIHUE POST	60
ILPC341U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	13	IOL20T	IOL ABUTMENT 2MM(H)	37,41
ILPC342	CERTAIN LOW PROFILE ABUTMENT 3.4MM(D) X 2MM(H)	13	IOL30T	IOL ABUTMENT 3MM(H)	37,41
ILPC342U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	13	IOL40T	IOL ABUTMENT 4MM(H)	37,41
ILPC343	CERTAIN LOW PROFILE ABUTMENT 3.4MM(D) X 3MM(H)	13	IOL55T	IOL ABUTMENT 5.5MM(H)	37,41
ILPC343U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	13	IOL70T	IOL ABUTMENT 7MM(H)	37,41
ILPC344	CERTAIN LOW PROFILE ABUTMENT 3.4MM(D) X 4MM(H)	13	IOLDE	IOL DISTAL EXTENSION	20,42
ILPC344U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	13	IOLGC	IOL GOLD CYLINDER	16,20,38,42
ILPC441	CERTAIN LOW PROFILE ABUTMENT 4.1MM(D) X 1MM(H)	13	IOLHC	IOL HEALING CAP	16,20,38,42
ILPC441U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	13	IOLLAS	IOL STRAIGHT LAB ANALOG	16,20,38,42
ILPC442	CERTAIN LOW PROFILE ABUTMENT 4.1MM(D) X 2MM(H)	13	IOLPIC	IOL PICK-UP IMPRESSION COPING	16,20,38,42
ILPC442U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	13	IOLPP	IOL POLISHING PROTECTOR	16,20,38,42
ILPC443	CERTAIN LOW PROFILE ABUTMENT 4.1MM(D) X 3MM(H)	13	IOLTIC	IOL TWIST LOCK™ IMPRESSION COPING	16,20,38,42
ILPC443U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	13	IOLTIC	IOL TRANSFER IMPRESSION COPING	16,20,38,42
ILPC444	CERTAIN LOW PROFILE ABUTMENT 4.1MM(D) X 4MM(H)	13	IPA4140	PROVIDE® ABUTMENT - 4.1MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	3
ILPC444U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	13	IPA4155	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	3
ILPC541	CERTAIN LOW PROFILE ABUTMENT 5.0MM(D) X 1MM(H)	13	IPA4240	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	3
ILPC541U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 1MM(H)	13	IPA4255	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	3
ILPC542	CERTAIN LOW PROFILE ABUTMENT 5.0MM(D) X 2MM(H)	13	IPA4340	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	3
ILPC542U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 2MM(H)	13			
ILPC543	CERTAIN LOW PROFILE ABUTMENT 5.0MM(D) X 3MM(H)	13			
ILPC543U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 3MM(H)	13			
ILPC544	CERTAIN LOW PROFILE ABUTMENT 5.0MM(D) X 4MM(H)	13			
ILPC544U	CERTAIN LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 4MM(H)	13			
ILRGHG	CERTAIN GOLD-TITE® (HEXED) LARGE SCREW	12,53			
ILRGHT	CERTAIN TITANIUM (HEXED) LARGE SCREW	12,53			
ILT150	CERTAIN LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE 4MM(D)	59			
ILTAH57	CERTAIN LABORATORY ABUTMENT HOLDER FOR ALL CERTAIN PLATFORMS	6,8,10,12,59			
IMAP32G	CERTAIN GINGIHUE® POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	5			
IMAP34G	CERTAIN GINGIHUE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	5			
IMCA31	CERTAIN CONICAL ABUTMENT 3.4MM(D) X 1MM(H)	17			
IMCA32	CERTAIN CONICAL ABUTMENT 3.4MM(D) X 2MM(H)	17			
IMCA33	CERTAIN CONICAL ABUTMENT 3.4MM(D) X 3MM(H)	17			

Index

Cat.#	Description	Page#	Cat.#	Description	Page#
IPA4355	PROVIDE® ABUTMENT - 4.1MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	3	IPAP662G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 2MM(H)	5
IPA4440	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 4.8MM(PROFILE)	3	IPAP664G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	5
IPA4455	PROVIDE ABUTMENT - 4.1MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 4.8MM(PROFILE)	3	IPAP672G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 2MM(H)	5
IPA5140	PROVIDE ABUTMENT - 5MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPAP674G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 4MM(H)	5
IPA5155	PROVIDE ABUTMENT - 5MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPAPF454	CERTAIN PERFORMANCE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	25
IPA5240	PROVIDE ABUTMENT - 5MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPAPF456	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 6MM(H)	25
IPA5255	PROVIDE ABUTMENT - 5MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPAPF554	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	25
IPA5340	PROVIDE ABUTMENT - 5MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPAPF556	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 6MM(H)	25
IPA5355	PROVIDE ABUTMENT - 5MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPAPF664	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	25
IPA5440	PROVIDE ABUTMENT - 5MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPAPF666	CERTAIN PERFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 6MM(H)	25
IPA5455	PROVIDE ABUTMENT - 5MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPFP454	CERTAIN PERFORMANCE POST 4.1MM(D) X 5MM(P) X 4MM(H)	25
IPA6140	PROVIDE ABUTMENT - 6MM(PLATFORM) X 1MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPFP456	CERTAIN PERFORMANCE POST 4.1MM(D) X 5MM(P) X 6MM(H)	25
IPA6155	PROVIDE ABUTMENT - 6MM(PLATFORM) X 1MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPFTC41	CERTAIN PERFORMANCE TEMPORARY CYLINDER 4.1MM (HEXED)	12,26
IPA6240	PROVIDE ABUTMENT - 6MM(PLATFORM) X 2MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPFTC42	CERTAIN PERFORMANCE TEMPORARY CYLINDER 4.1MM (NON-HEXED)	12,26
IPA6255	PROVIDE ABUTMENT - 6MM(PLATFORM) X 2MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPPIA3	CERTAIN UCLA POLISHING PROTECTOR 4.1MM(D)	59
IPA6340	PROVIDE ABUTMENT - 6MM(PLATFORM) X 3MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPPIA5	CERTAIN UCLA POLISHING PROTECTOR 5MM(D)	59
IPA6355	PROVIDE ABUTMENT - 6MM(PLATFORM) X 3MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IPPIA6	CERTAIN UCLA POLISHING PROTECTOR 6MM(D)	59
IPA6440	PROVIDE ABUTMENT - 6MM(PLATFORM) X 4MM(COLLAR) X 4MM(POST) X 6.5MM(PROFILE)	3	IPPM1	CERTAIN UCLA POLISHING PROTECTOR 3.4MM(D)	59
IPA6455	PROVIDE ABUTMENT - 6MM(PLATFORM) X 4MM(COLLAR) X 5.5MM(POST) X 6.5MM(PROFILE)	3	IQSA01	CERTAIN QUICKSEAT® ACTIVATOR TOOL	6,8,10,11,12
IPAP452G	CERTAIN® GINGIHUE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 2MM(H)	5	IRH600	CERTAIN REAMER WITH HANDLE	59
IPAP454G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	5	ISRT01	CERTAIN HAND TAP	59
IPAP462G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 2MM(H)	5	ISRT05	CERTAIN GUIDE HANDLE	59
IPAP464G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 4MM(H)	5	ISRT06	CERTAIN SCREW REMOVAL TOOL	59
IPAP472G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	5	ISRT07	MANUAL REVERSING TOOL	59
IPAP474G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	5	ISRT10	CERTAIN SCREW REMOVAL KIT	59
IPAP552G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 2MM(H)	5	ITCS41	TEMPORARY (HEXED) IMPLANT CYLINDER 4.1MM(D) W/RETENTION AND HEXED SCREW	34
IPAP554G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	5	ITCS42	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 4.1MM(D)	34
IPAP562G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 2MM(H)	5	IUNAB2C	CERTAIN UCLA CASTABLE NON-HEXED ABUTMENT CYLINDER 4.1MM(D)	11
IPAP564G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 4MM(H)	5	IUNAB2T	CERTAIN UCLA CASTABLE NON-HEXED ABUTMENT CYLINDER 4.1MM(D)	11
IPAP572G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 2MM(H)	5	IUNIHG	CERTAIN GOLD-TITE® (HEXED) SCREW	4,6,10,12,53
IPAP574G	CERTAIN GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 4MM(H)	5	IUNIHT	CERTAIN TITANIUM (HEXED) SCREW	4,6,10,12,53
			IUNITS	CERTAIN HEX TRY-IN SCREW (5PK) 3.4, 4.1, 5, 6MM(D)	6,10,12,53
			IWCA51	CERTAIN CONICAL ABUTMENT 5MM(D) X 1MM(H)	17
			IWCA52	CERTAIN CONICAL ABUTMENT 5MM(D) X 2MM(H)	17
			IWCA53	CERTAIN CONICAL ABUTMENT 5MM(D) X 3MM(H)	17
			IWCA54	CERTAIN CONICAL ABUTMENT 5MM(D) X 4MM(H)	17
			IWCA55	CERTAIN CONICAL ABUTMENT 5MM(D) X 5.5MM(H)	17
			IWCA61	CERTAIN CONICAL ABUTMENT 6MM(D) X 1MM(H)	17
			IWCA62	CERTAIN CONICAL ABUTMENT 6MM(D) X 2MM(H)	17
			IWCA63	CERTAIN CONICAL ABUTMENT 6MM(D) X 3MM(H)	17
			IWCA64	CERTAIN CONICAL ABUTMENT 6MM(D) X 4MM(H)	17
			IWCA65	CERTAIN CONICAL ABUTMENT 6MM(D) X 5.5MM(H)	17
			IWCAP564	CERTAIN ZIREAL® POST 5MM(D) X 6MM(P) X 4MM(H)	7
			IWCAP574	CERTAIN ZIREAL POST 5MM(D) X 7.5MM(P) X 4MM(H)	7
			IWGA51C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 5MM(D)	9,11
			IWGA52C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	11
			IWGA52T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	11
			IWGA61C	CERTAIN UCLA GOLD (HEXED) ABUTMENT CYLINDER 6MM(D)	9,11
			IWGA62C	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	11
			IWGA62T	CERTAIN UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	11
			IWIP50	CERTAIN STRAIGHT PICK-UP COPING 5MM(D) X 5MM(P)	6,8,10,12

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
IWIP55	CERTAIN® EP® PICK-UP COPING 5MM(D) X 5.6MM(P)	6,8,10,12	LOAD	LOCATOR BAR ATTACHMENT DRILL	22,24,44,46
IWIP56	CERTAIN EP PICK-UP COPING 5MM(D) X 6MM(P)	6,8,10,12	LOADT4	LOCATOR ABUTMENT DRIVER TIP 24MM(L)	24,46,56
IWIP57	CERTAIN EP PICK-UP COPING 5MM(D) X 7.5MM(P)	6,8,10,12	LOADT9	LOCATOR ABUTMENT DRIVER TIP 30MM(L)	24,46,56
IWIP60	CERTAIN STRAIGHT PICK-UP COPING 6MM(D) X 6MM(P)	6,10,12	LOAH	LOCATOR REPLACEMENT HOUSING	24,46
IWIP66	CERTAIN EP PICK-UP COPING 6MM(D) X 6.6MM(P)	6,10,12	LOAT	LOCATOR BAR ATTACHMENT TAP	22,24,44,46
IWIP67	CERTAIN EP PICK-UP COPING 6MM(D) X 7.5MM(P)	6,10,12	LORHK	LOCATOR REPLACEMENT HOUSING KIT	24,46
IWIT50	CERTAIN STRAIGHT TRANSFER COPING 5MM(D) X 5MM(P)	6,8,10,12	LPAC3217	LOW PROFILE 17° ABUTMENT 3.4MM(D) X 2MM(H)	35
IWIT55	CERTAIN EP TWIST LOCK™ COPING 5MM(D) X 5.6MM(P)	6,8,10,12	LPAC3330	LOW PROFILE 30° ABUTMENT 3.4MM(D) X 3MM(H)	35
IWIT56	CERTAIN EP TWIST LOCK COPING 5MM(D) X 6MM(P)	6,8,10,12	LPAC3417	LOW PROFILE 17° ABUTMENT 3.4MM(D) X 4MM(H)	35
IWIT57	CERTAIN EP TWIST LOCK COPING 5MM(D) X 7.5MM(P)	6,8,10,12	LPAC3530	LOW PROFILE 30° ABUTMENT 3.4MM(D) X 5MM(H)	35
IWIT60	CERTAIN STRAIGHT TRANSFER COPING 6MM(D) X 6MM(P)	6,10,12	LPAC4217	LOW PROFILE 17° ABUTMENT 4.1MM(D) X 2MM(H)	35
IWIT66	CERTAIN EP TWIST LOCK COPING 6MM(D) X 6.6MM(P)	6,10,12	LPAC4330	LOW PROFILE 30° ABUTMENT 4.1MM(D) X 3MM(H)	35
IWIT67	CERTAIN EP TWIST LOCK COPING 6MM(D) X 7.5MM(P)	6,10,12	LPAC4417	LOW PROFILE 17° ABUTMENT 4.1MM(D) X 4MM(H)	35
IWPC52C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D)11		LPAC4530	LOW PROFILE 30° ABUTMENT 4.1MM(D) X 5MM(H)	35
IWPC52T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D)11		LPAC5217	LOW PROFILE 17° ABUTMENT 5.0MM(D) X 2MM(H)	35
IWPC62C	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D)11		LPAC5330	LOW PROFILE 30° ABUTMENT 5.0MM(D) X 3MM(H)	35
IWPC62T	CERTAIN UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D) 11		LPAC5417	LOW PROFILE 17° ABUTMENT 5.0MM(D) X 4MM(H)	35
IWPP554	CERTAIN PREFORMANCE® POST 5MM(D) X 5MM(P) X 4MM(H)	25	LPAC541U	LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 1MM(H)	35
IWPP556	CERTAIN PREFORMANCE POST 5MM(D) X 5MM(P) X 6MM(H)	25	LPAC5530	LOW PROFILE 30° ABUTMENT 5.0MM(D) X 5MM(H)	35
IWPP664	CERTAIN PREFORMANCE POST 6MM(D) X 6MM(P) X 4MM(H)	25	LPC341	LOW PROFILE ABUTMENT 3.4MM(D) X 1MM(H)	35
IWPP666	CERTAIN PREFORMANCE POST 6MM(D) X 6MM(P) X 6MM(H)	25	LPC341U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 1MM(H)	35
IWPFCT51	CERTAIN PREFORMANCE TEMPORARY CYLINDER 5MM (HEXED)	12,26	LPC342	LOW PROFILE ABUTMENT 3.4MM(D) X 2MM(H)	35
IWPFCT52	CERTAIN PREFORMANCE TEMPORARY CYLINDER 5MM (NON-HEXED)	12,26	LPC342U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 2MM(H)	35
IWPFCT61	CERTAIN PREFORMANCE TEMPORARY CYLINDER 6MM (HEXED)	12,26	LPC343	LOW PROFILE ABUTMENT 3.4MM(D) X 3MM(H)	35
IWPFCT62	CERTAIN PREFORMANCE TEMPORARY CYLINDER 6MM (NON-HEXED)	12,26	LPC343U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 3MM(H)	35
IWPP552G	CERTAIN GINGIHUE® POST 5MM(D) X 5MM(P) X 2MM(H)	5	LPC344	LOW PROFILE ABUTMENT 3.4MM(D) X 4MM(H)	35
IWPP554G	CERTAIN GINGIHUE POST 5MM(D) X 5MM(P) X 4MM(H)	5	LPC344U	LOW PROFILE ONE-PIECE ABUTMENT 3.4MM(D) X 4MM(H)	35
IWPP562G	CERTAIN GINGIHUE POST 5MM(D) X 6MM(P) X 2MM(H)	5	LPC441	LOW PROFILE ABUTMENT 4.1MM(D) X 1MM(H)	35
IWPP564G	CERTAIN GINGIHUE POST 5MM(D) X 6MM(P) X 4MM(H)	5	LPC441U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 1MM(H)	35
IWPP572G	CERTAIN GINGIHUE POST 5MM(D) X 7.5MM(P) X 2MM(H)	5	LPC442	LOW PROFILE ABUTMENT 4.1MM(D) X 2MM(H)	35
IWPP574G	CERTAIN GINGIHUE POST 5MM(D) X 7.5MM(P) X 4MM(H)	5	LPC442U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 2MM(H)	35
IWPP662G	CERTAIN GINGIHUE POST 6MM(D) X 6MM(P) X 2MM(H)	5	LPC443	LOW PROFILE ABUTMENT 4.1MM(D) X 3MM(H)	35
IWPP664G	CERTAIN GINGIHUE POST 6MM(D) X 6MM(P) X 4MM(H)	5	LPC443U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 3MM(H)	35
IWPP672G	CERTAIN GINGIHUE POST 6MM(D) X 7.5MM(P) X 2MM(H)	5	LPC444	LOW PROFILE ABUTMENT 4.1MM(D) X 4MM(H)	35
IWPP674G	CERTAIN GINGIHUE POST 6MM(D) X 7.5MM(P) X 4MM(H)	5	LPC444U	LOW PROFILE ONE-PIECE ABUTMENT 4.1MM(D) X 4MM(H)	35
IWSU30	CERTAIN WAXING SCREW/GUIDE PIN	53,59	LPC541	LOW PROFILE ABUTMENT 5.0MM(D) X 1MM(H)	35
IWTCS51	CERTAIN TEMPORARY (HEXED) CYLINDER 5MM(D) W/HEXED SCREW	12	LPC542	LOW PROFILE ABUTMENT 5.0MM(D) X 2MM(H)	35
IWTCS52	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 5MM(D) W/LARGE DIA. SCREW	12	LPC542U	LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 2MM(H)	35
IWTCS61	CERTAIN TEMPORARY (HEXED) CYLINDER 6MM(D) W/HEXED SCREW	12	LPC543	LOW PROFILE ABUTMENT 5.0MM(D) X 3MM(H)	35
IWTCS62	CERTAIN TEMPORARY (NON-HEXED) CYLINDER 6MM(D) W/LARGE DIA. SCREW	12	LPC543U	LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 3MM(H)	35
IZIRTS	CERTAIN HEX TRY-IN SCREW	8	LPC544	LOW PROFILE ABUTMENT 5.0MM(D) X 4MM(H)	35
IZSHG	CERTAIN ZIREAL® GOLD-TITE® (HEXED) SCREW	8,53	LPC544U	LOW PROFILE ONE-PIECE ABUTMENT 5.0MM(D) X 4MM(H)	35
LAELM	LOCATOR® EXTRA LIGHT RETENTION MALES (4PK)	24,46	LPCAM1	LOW PROFILE ABUTMENT LAPPING TOOL	14,36
LAERM	LOCATOR EXTENDED RANGE MALES - GREEN, 4LBS/1800G (4PK)	24	LPCCC1	LOW PROFILE ABUTMENT (HEXED) CASTABLE CYLINDER	14,36
LAIC1	LOCATOR ABUTMENT IMPRESSION COPING	24,46	LPCCC2	LOW PROFILE ABUTMENT (NON-HEXED) CASTABLE CYLINDER	14,36
LALA1	LOCATOR ABUTMENT LAB ANALOG	24,46	LPCDE	LOW PROFILE ABUTMENT DISTAL EXTENSION	14,36
LARMS	LOCATOR REPLACEMENT MALES - WHITE, 5LBS/2250G (4PK)	24,46	LPCGC1	LOW PROFILE ABUTMENT (HEXED) GOLD CYLINDER	14,36
LCTDR1	LOCATOR CORE TOOL/ABUTMENT DRIVER	24,46	LPCGC2	LOW PROFILE ABUTMENT (NON-HEXED) GOLD CYLINDER	14,36
LELARM	EXTRA LIGHT RETENTION EXTENDED RANGE MALES - RED, 1.5LBS/680G	24,46	LPCGSH	LOW PROFILE ABUTMENT GOLD-TITE RETAINING SCREW	14,36
LLRMS	LOCATOR LIGHT RETENTION REPLACEMENT MALES - PINK, 3LBS/1350G (4PK)	24,46	LPCHC	LOW PROFILE ABUTMENT HEALING CAP	14,36
LOA001	LOCATOR ABUTMENT 4.1MM(D) X 1MM(H)	45	LPCLA	LOW PROFILE ABUTMENT LAB ANALOG	14,36
LOA002	LOCATOR ABUTMENT 4.1MM(D) X 2MM(H)	45	LPCPIC1	LOW PROFILE ABUTMENT (HEXED) PICK-UP IMPRESSION COPING	144,36
LOA003	LOCATOR ABUTMENT 4.1MM(D) X 3MM(H)	45	LPCPIC2	LOW PROFILE ABUTMENT (NON-HEXED) PICK-UP IMPRESSION COPING	16,36
LOA004	LOCATOR ABUTMENT 4.1MM(D) X 4MM(H)	45	LPCPP	LOW PROFILE ABUTMENT POLISHING PROTECTOR	16,36
LOA005	LOCATOR ABUTMENT 4.1MM(D) X 5MM(H)	45	LPCPTC1	LOW PROFILE ABUTMENT (HEXED) PREFORMANCE TEMPORARY CYLINDER	16,36
LOA006	LOCATOR ABUTMENT 4.1MM(D) X 6MM(H)	45	LPCPTC2	LOW PROFILE ABUTMENT (NON-HEXED) PREFORMANCE TEMPORARY CYLINDER	16,36
LOAB	LOCATOR BAR ATTACHMENT	22,24,44,46	LPCQB	LOW PROFILE ABUTMENT QUICKBRIDGE®	16,36
			LPCQBAP	LOW PROFILE ABUTMENT QUICKBRIDGE REPLACEMENT CAP	16,36

Index

Cat.#	Description	Page#	Cat.#	Description	Page#
LPCRIC	LOW PROFILE ABUTMENT QUICKBRIDGE IMPRESSION COPING	14,36	NCATD0	CONTRA ANGLE TORQUE DRIVER KIT	55
LPCTC1	LOW PROFILE ABUTMENT (HEXED) TEMPORARY CYLINDER	14,36	NCATD0C	CONTRA ANGLE TORQUE DRIVER KIT CERTAIN	55
LPCTC2	LOW PROFILE ABUTMENT (NON-HEXED) TEMPORARY CYLINDER	14,36	NPSDK0	PROSTHETIC DRIVER KIT	55
LPCTIC1	LOW PROFILE ABUTMENT (HEXED) TRANSFER IMPRESSION COPING	14,36	NTMOD1	3X MODEL OF OSSEOTITE® TAPERED IMPLANT	60
LPCTIC2	LOW PROFILE ABUTMENT (NON-HEXED) TRANSFER IMPRESSION COPING	14,36	ORCG1	GOLD HADER CLIP	22,44
LPCTSH	LOW PROFILE ABUTMENT TITANIUM RETAINING SCREW	14,36	ORCY1	PLASTIC HADER CLIP	22,44
LPCTUCA	LOW PROFILE ABUTMENT LASER WELD CYLINDER	14,36	ORLAU	UNIVERSAL O-RING ABUTMENT LAB ANALOG	48
LPCWS	LOW PROFILE ABUTMENT WAXING SCREW	14,36	OSO20	O-RING ABUTMENT 4.1MM(D) X 2MM(H)	47
LT150	LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE, 4MM(D)	59	OSO40	O-RING ABUTMENT 4.1MM(D) X 4MM(H)	47
LTAH5	LABORATORY ABUTMENT HOLDER FOR 3.4MM(D)	28,32,34,59	OSO60	O-RING ABUTMENT 4.1MM(D) X 6MM(H)	47
LTAH7	LABORATORY HOLDER FOR 4.1, 5, 6MM(D)	28,30,32,34,59	OSOBK	O-RING REPLACEMENTS	48
L-TIRW	LOW TORQUE INDICATING RATCHET WRENCH	55	OSOCA	O-RING CASTABLE SYSTEM	48
MAP32G	GINGIHUE® POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	27	OSODH	O-RING HOUSING	48
MAP34G	GINGIHUE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	27	OSORED	RED PROCESSING O-RING	48
MCA31	CONICAL ABUTMENT 3.4MM(D) X 1MM(H)	39	OSSMOD1	3X MODEL OF OSSEOTITE IMPLANT 4MM(D) X 13MM(L)	60
MCA32	CONICAL ABUTMENT 3.4MM(D) X 2MM(H)	39	PAA484	PROVIDE® ABUTMENT ANALOG 4.8MM(P) X 4MM(H)	4
MCA33	CONICAL ABUTMENT 3.4MM(D) X 3MM(H)	39	PAA485	PROVIDE ABUTMENT ANALOG 4.8MM(P) X 5.5MM(H)	4
MCA34	CONICAL ABUTMENT 3.4MM(D) X 4MM(H)	39	PAA654	PROVIDE ABUTMENT ANALOG 6.5MM(P) X 4MM(H)	4
MCAG1	CONICAL GOLD CYLINDER (HEXED) 3.4MM(D)	18,40	PAA655	PROVIDE ABUTMENT ANALOG 6.5MM(P) X 5.5MM(H)	4
MCAG2	CONICAL GOLD CYLINDER (NON-HEXED) 3.4MM(D)	18,40	PAAP48	PROVIDE ABUTMENT ANALOG WITH PIN 4.8MM(P)	4
MCTC1	CONICAL ABUTMENT TEMPORARY CYLINDER (HEXED) 3.4MM(D)	18,40	PAAP65	PROVIDE ABUTMENT ANALOG WITH PIN 6.5MM(P)	4
MCTC2	CONICAL ABUTMENT TEMPORARY 3.4MM(D) CYLINDER (NON-HEXED)	18,40	PAD00	POSTERIOR ABUTMENT DRIVER 17MM(L)	16,20,38,42,55,56
MEC33	CONICAL ABUTMENT PICK-UP COPING 3.4MM(D)	18,40	PAD01	O-RING/DAL-RO ABUTMENT DRIVER 24MM(L)	50,56
MHC33	CONICAL HEALING CAP 3.4MM(D)	18,40	PAD24	STANDARD ABUTMENT DRIVER 24MM(L)	16,20,38,55,56
MIC33	PICK UP IMPRESSION COPING 3.4MM(D)	28,32,34	PAK4140	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 1MM(H) - 4MM POST	3
MIDTH	MANUAL INTERCHANGEABLE DRIVER TIP HANDLE	56	PAK4155	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 1MM(H) - 5.5MM POST	3
MLOA001	LOCATOR® ABUTMENT 3.4MM(D) X 1MM(H)	45	PAK4240	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 2MM(H) - 4MM POST	3
MLOA002	LOCATOR ABUTMENT 3.4MM(D) X 2MM(H)	45	PAK4255	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 2MM(H) - 5.5MM POST	3
MLOA003	LOCATOR ABUTMENT 3.4MM(D) X 3MM(H)	45	PAK4340	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 3MM(H) - 4MM POST	3
MLOA004	LOCATOR ABUTMENT 3.4MM(D) X 4MM(H)	45	PAK4355	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 3MM(H) - 5.5MM POST	3
MLOA005	LOCATOR ABUTMENT 3.4MM(D) X 5MM(H)	45	PAK4440	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 4MM(H) - 4MM POST	3
MLOA006	LOCATOR ABUTMENT 3.4MM(D) X 6MM(H)	45	PAK4455	PROVIDE ABUTMENT PLACEMENT KIT 4.1MM(D) X 4.8MM(P) X 4MM(H) - 5.5MM POST	3
MLT150	LAPPING TOOL FOR CASTABLE UCLA ABUTMENT W/GUIDE, 3.4MM(D)	59	PAK5140	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 1MM(H) - 4MM POST	3
MMCLA	CONICAL LAB ANALOG 3.4MM(D)	18,40	PAK5155	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 1MM(H) - 5.5MM POST	3
MMILA	LAB ANALOG 3.4MM(D)	28,32,34	PAK5240	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 2MM(H) - 4MM POST	3
MMTCS1	TEMPORARY (HEXED) CYLINDER 3.4MM(D) W/RETENTION AND (HEXED) SCREW	34	PAK5255	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 2MM(H) - 5.5MM POST	3
MODWRENCH	WRENCH FOR TIGHTENING MODEL SCREWS	60	PAK5340	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 3MM(H) - 4MM POST	3
MPAP32G	GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 2MM(H)	27	PAK5355	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 6.5MM(P) X 3MM(H) - 5.5MM POST	3
MPAP34G	GINGIHUE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	27	PAK5440	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 4MM(H) - 4MM POST	3
MPAPF34	PREFORMANCE® 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	51	PAK5455	PROVIDE ABUTMENT PLACEMENT KIT 5MM(D) X 4.8MM(P) X 4MM(H) - 5.5MM POST	3
MPAPF36	PREFORMANCE 15° PRE-ANGLED POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	51	PAK6140	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 1MM(H) - 4MM POST	3
MPFP34	PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 4MM(H)	51	PAK6155	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 1MM(H) - 5.5MM POST	3
MPFP36	PREFORMANCE POST 3.4MM(D) X 3.8MM(P) X 6MM(H)	51			
MPFTC32	PREFORMANCE TEMPORARY CYLINDER 3.4MM (NON-HEXED)	34			
MPFTC34	PREFORMANCE TEMPORARY CYLINDER 3.4MM (HEXED)	34			
MSGIAM1	NAVIGATOR® CERTAIN® ANALOG MOUNT, 3.4MM(D) X 1(L)	58			
MSGIAM2	NAVIGATOR CERTAIN ANALOG MOUNT, 3.4MM(D) X 2(L)	58			
MSGIAM3	NAVIGATOR CERTAIN ANALOG MOUNT, 3.4MM(D) X 3(L)	58			
MSGIAM4	NAVIGATOR CERTAIN ANALOG MOUNT, 3.4MM(D) X 4(L)	58			
MUCC2C	UCLA CASTABLE NON-HEXED ABUTMENT CYLINDER 3.4MM(D)	33			
MUCG1C	UCLA GOLD HEXED ABUTMENT CYLINDER 3.4MM(D)	33			
MUCG2C	UCLA GOLD NON-HEXED ABUTMENT CYLINDER 3.4MM(D)	33			
MUNITS	SQUARE TRY-IN SCREW, 3.4MM(D) (5PK)	28,32,54			

Index

Cat.#	Description	Page#	Cat.#	Description	Page#
PAK6240	PROVIDE® ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 2MM(H) - 4MM POST	3	PRK484	PROVIDE ABUTMENT RESTORATIVE KIT 4.8MM(P) - 4MM POST	3
PAK6255	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 2MM(H) - 5.5MM POST	3	PRK485	PROVIDE ABUTMENT RESTORATIVE KIT 4.8MM(P) - 5.5MM POST	3
PAK6340	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 3MM(H) - 4MM POST	3	PRK654	PROVIDE ABUTMENT RESTORATIVE KIT 6.5MM(P) - 4MM POST	3
PAK6355	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 3MM(H) - 5.5MM POST	3	PRK655	PROVIDE ABUTMENT RESTORATIVE KIT 6.5MM(P) - 5.5MM POST	3
PAK6440	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 4MM(H) - 4MM POST	3	PSD00	POSTERIOR SLOTTED SCREW DRIVER - SLOTTED 17MM(L)	55
PAK6455	PROVIDE ABUTMENT PLACEMENT KIT 6MM(D) X 6.5MM(P) X 4MM(H) - 5.5MM POST	3	PSD01	STANDARD SLOTTED SCREW DRIVER - SLOTTED 24MM(L)	55
PAP452G	GINGIHUE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 2MM(H)	27	PSDT1	PROSTHETIC SYSTEM DRIVER TRAY	55
PAP454G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	27	PSQD0N	NARROW POSTERIOR SQUARE DRIVER 17MM(L)	54,55,56
PAP462G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 2MM(H)	27	PSQD1N	NARROW STANDARD SLOTTED SQUARE DRIVER 24MM(L)	54,55,56
PAP464G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 6MM(P) X 4MM(H)	27	PTC345	PREP-TITE® CAP 5MM: USE WITH MAP32G, MAP34G	5
PAP472G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 2MM(H)	27	PTC347	PREP-TITE CAP 7MM: USE WITH MAP32G, MAP34G	5
PAP474G	GINGIHUE 15° PRE-ANGLED POST 4.1MM(D) X 7.5MM(P) X 4MM(H)	27	PTC455	PREP-TITE CAP 5MM: USE WITH APP452G, APP454G	5
PAP552G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 2MM(H)	27	PTC457	PREP-TITE CAP 7MM: USE WITH APP452G, APP454G	5
PAP554G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	27	PTC465	PREP-TITE CAP 5MM: USE WITH APP462G, APP464G, WPP562G, WPP564G	5
PAP562G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 2MM(H)	27	PTC467	PREP-TITE CAP 7MM: USE WITH APP462G, APP464G, WPP562G, WPP564G	5
PAP564G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 6MM(P) X 4MM(H)	27	PTC475	PREP-TITE CAP 5MM: USE WITH APP472G, APP474G, WPP572G, WPP574G, WPP672G, WPP674G	5
PAP572G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 2MM(H)	27	PTC477	PREP-TITE CAP 7MM: USE WITH APP472G, APP474G, WPP572G, WPP574G, WPP672G, WPP674G	5
PAP574G	GINGIHUE 15° PRE-ANGLED POST 5MM(D) X 7.5MM(P) X 4MM(H)	27	PTC555	PREP-TITE CAP 5MM: USE WITH WPP552G, WPP554G	5
PAP662G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 2MM(H)	27	PTC557	PREP-TITE CAP 7MM: USE WITH WPP552G, WPP554G	5
PAP664G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	27	PTC665	PREP-TITE CAP 5MM: USE WITH WPP662G, WPP664G	5
PAP672G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 2MM(H)	27	PTC667	PREP-TITE CAP 7MM: USE WITH WPP662G, WPP664G	5
PAP674G	GINGIHUE 15° PRE-ANGLED POST 6MM(D) X 7.5MM(P) X 4MM(H)	27	PUA48M	PROVIDE TEMPORARY CYLINDER MULTI-UNIT - 4.8MM PROFILE	4
PAPF454	PREFORMANCE® 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 4MM(H)	51	PUA48S	PROVIDE TEMPORARY CYLINDER SINGLE-UNIT - 4.8MM PROFILE	4
PAPF456	PREFORMANCE 15° PRE-ANGLED POST 4.1MM(D) X 5MM(P) X 6MM(H)	51	PUA65M	PROVIDE TEMPORARY CYLINDER MULTI-UNIT - 6.5MM PROFILE	4
PAPF554	PREFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 4MM(H)	51	PUA65S	PROVIDE TEMPORARY CYLINDER SINGLE-UNIT - 6.5MM PROFILE	4
PAPF556	PREFORMANCE 15° PRE-ANGLED POST 5MM(D) X 5MM(P) X 6MM(H)	51	PWS48M	PROVIDE WAXING SLEEVE 4.8MM(P) MULTI-UNIT	4
PAPF664	PREFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 4MM(H)	51	PWS48S	PROVIDE WAXING SLEEVE 4.8MM(P) SINGLE-UNIT	4
PAPF666	PREFORMANCE 15° PRE-ANGLED POST 6MM(D) X 6MM(P) X 6MM(H)	51	PWS65M	PROVIDE WAXING SLEEVE 6.5MM(P) MULTI-UNIT	4
PEMODLOC	PATIENT ED MODEL - LOCATOR®	60	PWS65S	PROVIDE WAXING SLEEVE 6.5MM(P) SINGLE-UNIT	4
PEMODSM	PATIENT ED MODEL - SINGLE/MULTIPLE TEETH	60	QKBRG	QUICKBRIDGE®	18,40
PPF454	PREFORMANCE POST 4.1MM(D) X 5MM(P) X 4MM(H)	51	RAOR1	RIGHT ANGLE O-RING/DAL-RO ABUTMENT DRIVER TIP	48,50,56
PPF456	PREFORMANCE POST 4.1MM(D) X 5MM(P) X 6MM(H)	51	RASA3	RIGHT ANGLE ABUTMENT DRIVER TIP - STEEL	16,20,38,42,55,56
PFTC41	PREFORMANCE TEMPORARY CYLINDER 4.1MM (HEXED)	34,52	RASD1	RIGHT ANGLE SLOTTED DRIVER TIP 24MM(L)	55
PFTC42	PREFORMANCE TEMPORARY CYLINDER 4.1MM (NON-HEXED)	34,52	RASD6	RIGHT ANGLE SLOTTED DRIVER TIP 30MM(L)	55
PHD00N	NARROW POSTERIOR SMALL HEX DRIVER 17MM(L)	56	RASH2N	NARROW RIGHT ANGLE SMALL HEX DRIVER TIP 24MM(L)	56
PHD01N	NARROW STANDARD SMALL HEX DRIVER 24MM(L)	56	RASH3N	NARROW RIGHT ANGLE LARGE HEX DRIVER TIP 24MM(L)	53,54,55,56
PHD02N	NARROW POSTERIOR LARGE HEX DRIVER 17MM(L)	53,54,55,56	RASH4	RIGHT ANGLE DRIVER TIP 50 IN. HEX 24MM(L)	24,46,56
PHD03N	NARROW STANDARD LARGE HEX DRIVER 24MM(L)	53,54,55,56	RASH7N	NARROW RIGHT ANGLE SMALL HEX DRIVER TIP 30MM(L)	56
PIC484	PROVIDE IMPRESSION COPING 4.8MM(P) X 4MM(H)	4	RASH8N	NARROW RIGHT ANGLE LARGE HEX DRIVER TIP 30MM(L)	53,54,55,56
PIC484H	PROVIDE IMPRESSION COPING WITH HOLES 4.8MM(P) X 4MM(H)	4	RASH9	RIGHT ANGLE DRIVER TIP 50 IN. HEX 30MM(L)	24,46,56
PIC485	PROVIDE IMPRESSION COPING 4.8MM(P) X 5.5MM(H)	4	RASQ3N	NARROW RIGHT ANGLE SQUARE DRIVER TIP 24MM(L)	54,55,56
PIC485H	PROVIDE IMPRESSION COPING WITH HOLES 4.8MM(P) X 5.5MM(H)	4	RASQ8N	NARROW RIGHT ANGLE SQUARE DRIVER TIP 30MM(L)	54,55,56
PIC654	PROVIDE IMPRESSION COPING 6.5MM(P) X 4MM(H)	4	RH600	REAMER/HANDLE FOR SGC34, UNAB1/2	59
PIC654H	PROVIDE IMPRESSION COPING WITH HOLES 6.5MM(P) X 4MM(H)	4	RTI2035TR	RESTORATIVE TORQUE INDICATOR TRAY	55
PIC655	PROVIDE IMPRESSION COPING 6.5MM(P) X 5.5MM(H)	4	SCA001	CONICAL ABUTMENT GOLD STANDARD ZR™ 4.1MM(D) X 1MM(H)	39
PIC655H	PROVIDE IMPRESSION COPING WITH HOLES 6.5MM(P) X 5.5MM(H)	4	SCA002	CONICAL ABUTMENT GOLD STANDARD ZR 4.1MM(D) X 2MM(H)	39
PPC484	PROVIDE PROTECTION CAP 4.8MM(P) X 4MM(H)	4	SCA003	CONICAL ABUTMENT GOLD STANDARD ZR 4.1MM(D) X 3MM(H)	39
PPC485	PROVIDE PROTECTION CAP 4.8MM(P) X 5.5MM(H)	4	SCA004	CONICAL ABUTMENT GOLD STANDARD ZR 4.1MM(D) X 4MM(H)	39
PPC654	PROVIDE PROTECTION CAP 6.5MM(P) X 4MM(H)	4	SCA055	CONICAL ABUTMENT GOLD STANDARD ZR 4.1MM(D) X 5.5MM(H)	39
PPC655	PROVIDE PROTECTION CAP 6.5MM(P) X 5.5MM(H)	4	SGC30	CHAMFERED GOLD CYLINDER FOR STANDARD ABUTMENT	22,44
PPCA3	POLISHING PROTECTOR CONICAL ABUTMENT 4.1 & 5MM(D)	18,40	SGC34	STANDARD ABUTMENT CASTABLE PLASTIC CYLINDER	22,44
PPIA3	POLISHING PROTECTOR UCLA ABUTMENT 4.1MM(D)	59	SGIAM41	NAVIGATOR® CERTAIN® ANALOG MOUNT, 4.1MM(D) X 1(L)	58
PPMC1	POLISHING PROTECTOR - CONICAL ABUTMENT 3.4MM(D)	18,40,59	SGIAM42	NAVIGATOR CERTAIN ANALOG MOUNT, 4.1MM(D) X 2(L)	58
PPMM1	POLISHING PROTECTOR UCLA 3.4MM(D)	59	SGIAM43	NAVIGATOR CERTAIN ANALOG MOUNT, 4.1MM(D) X 3(L)	58
PPSA3	POLISHING PROTECTOR STANDARD ABUTMENT	22,44,59	SGIAM44	NAVIGATOR CERTAIN ANALOG MOUNT, 4.1MM(D) X 4(L)	58
			SGIAM51	NAVIGATOR CERTAIN ANALOG MOUNT, 5MM(D) X 1(L)	58
			SGIAM52	NAVIGATOR CERTAIN ANALOG MOUNT, 5MM(D) X 2(L)	58
			SGIAM53	NAVIGATOR CERTAIN ANALOG MOUNT, 5MM(D) X 3(L)	58
			SGIAM54	NAVIGATOR CERTAIN ANALOG MOUNT, 5MM(D) X 4(L)	58

Index

Cat. #	Description	Page#	Cat. #	Description	Page#
SGLKIT	NAVIGATOR® LABORATORY KIT	58	WGA52C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	33
SGLTRAY	NAVIGATOR LABORATORY TRAY	58	WGA61C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 6MM(D)	31,33
SGUCA1C	UCLA GOLD STANDARD ZR™ (HEXED) ABUTMENT CYLINDER 4.1MM(D)	31,33	WGA62C	UCLA GOLD (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	33
SIC70	TWIST LOCK™ IMPRESSION COPING	22,44	WIP55	IMPLANT EP PICK-UP COPING 5MM(D) X 5MM(P)	28,30,32,34
SLA20	STANDARD ABUTMENT LAB ANALOG (STAINLESS)	22,44	WIP56	IMPLANT EP PICK-UP COPING 5MM(D) X 6MM(P)	28,30,32,34
SQIC7	PICK-UP IMPRESSION COPING	22,44	WIP57	IMPLANT EP PICK-UP COPING 5MM(D) X 7.5MM(P)	28,30,32,34
SRT01	HAND TAP FOR SRT10	59	WIP66	IMPLANT EP PICK-UP COPING 6MM(D) X 6MM(P)	28,32,34
SRT02	HAND DRILL 14MM(D) BRONZE DRILL FOR SRT10	59	WIP67	IMPLANT EP PICK-UP COPING 6MM(D) X 7.5MM(P)	28,32,34
SRT03	HAND DRILL 1.18MM(D) SILVER DRILL FOR SRT10	59	WIT55	IMPLANT EP TWIST LOCK COPING 5MM(D) X 5MM(P)	28,30,32,34
SRT04	EXTRACTING DRILL - ISO LATCH FOR SRT10	59	WIT56	IMPLANT EP TWIST LOCK COPING 5MM(D) X 6MM(P)	28,30,32,34
SRT05	GUIDE HANDLE FOR SRT10	59	WIT57	IMPLANT EP TWIST LOCK COPING 5MM(D) X 7.5MM(P)	28,30,32,34
SRT10	SCREW REMOVING KIT	59	WIT66	IMPLANT EP TWIST LOCK COPING 6MM(D) X 6MM(P)	28,32,34
SWCA51	CONICAL ABUTMENT GOLD STANDARD ZR 5MM(D) X 1MM(H)	39	WIT67	IMPLANT EP TWIST LOCK COPING 6MM(D) X 7.5MM(P)	28,32,34
SWCA52	CONICAL ABUTMENT GOLD STANDARD ZR 5MM(D) X 2MM(H)	39	WLT10	UCLA WIDE DIAMETER	59
SWCA53	CONICAL ABUTMENT GOLD STANDARD ZR 5MM(D) X 3MM(H)	39	WOSO20	O-RING ABUTMENT 5MM(D) X 2MM(H)	47
SWCA54	CONICAL ABUTMENT GOLD STANDARD ZR 5MM(D) X 4MM(H)	39	WOSO40	O-RING ABUTMENT 5MM(D) X 4MM(H)	47
SWCA55	CONICAL ABUTMENT GOLD STANDARD ZR 5MM(D) X 5.5MM(H)	39	WOSO60	O-RING ABUTMENT 5MM(D) X 6MM(H)	47
SWCA61	CONICAL ABUTMENT GOLD STANDARD ZR 6MM(D) X 1MM(H)	39	WPC51C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER 5MM(D)	31,33
SWCA62	CONICAL ABUTMENT GOLD STANDARD ZR 6MM(D) X 2MM(H)	39	WPC52C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 5MM(D)	33
SWCA63	CONICAL ABUTMENT GOLD STANDARD ZR 6MM(D) X 3MM(H)	39	WPC61C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER 6MM(D)	31,33
SWCA64	CONICAL ABUTMENT GOLD STANDARD ZR 6MM(D) X 4MM(H)	39	WPC62C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER 6MM(D)	33
SWCA65	CONICAL ABUTMENT GOLD STANDARD ZR 6MM(D) X 5.5MM(H)	39	WPP554	PREFORMANCE® POST 5MM(D) X 5MM(P) X 4MM(H)	51
SWGA51C	UCLA GOLD STANDARD ZR (HEXED) ABUTMENT CYLINDER 5MM(D)	31,33	WPP556	PREFORMANCE POST 5MM(D) X 5MM(P) X 6MM(H)	51
SWGA61C	UCLA GOLD STANDARD ZR (HEXED) ABUTMENT CYLINDER 6MM(D)	31,33	WPP664	PREFORMANCE POST 6MM(D) X 6MM(P) X 4MM(H)	51
TC300	STANDARD ABUTMENT TEMPORARY CYLINDER	22,44	WPP666	PREFORMANCE POST 6MM(D) X 6MM(P) X 6MM(H)	51
TD-10	CONTRA ANGLE TORQUE CONTROLLER 10NCM	55	WPFTC51	PREFORMANCE TEMPORARY CYLINDER 5MM (HEXED)	34,52
TD-20	CONTRA ANGLE TORQUE CONTROLLER 20NCM	55	WPFTC52	PREFORMANCE TEMPORARY CYLINDER 5MM (NON-HEXED)	34,52
TD-35	CONTRA ANGLE TORQUE CONTROLLER 32NCM	55	WPFTC61	PREFORMANCE TEMPORARY CYLINDER 6MM (HEXED)	34,52
THRC4	TEMPORARY HEALING RETENTION CYLINDER 4.1MM(D) X 4MM(H)	43,45,47,49	WPFTC62	PREFORMANCE TEMPORARY CYLINDER 6MM (NON-HEXED)	34,52
THRC6	TEMPORARY HEALING RETENTION CYLINDER 4.1MM(D) X 6MM(H)	43,45,47,49	WPP50	POLISHING PROTECTOR 5MM(D)	59
UNA125	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER (25PK)	31,33	WPP552G	GINGIHUE® POST 5MM(D) X 5MM(P) X 2MM(H)	27
UNA225	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER (25PK)	33	WPP554G	GINGIHUE POST 5MM(D) X 5MM(P) X 4MM(H)	27
UNAB1C	UCLA CASTABLE (HEXED) ABUTMENT CYLINDER	31,33	WPP562G	GINGIHUE POST 5MM(D) X 6MM(P) X 2MM(H)	27
UNAB2C	UCLA CASTABLE (NON-HEXED) ABUTMENT CYLINDER	33	WPP564G	GINGIHUE POST 5MM(D) X 6MM(P) X 4MM(H)	27
UNIHG	GOLD-TITE® (HEXED) SCREW	28,30,32,34,54	WPP572G	GINGIHUE POST 5MM(D) X 7.5MM(P) X 2MM(H)	27
UNIHT	TITANIUM (HEXED) SCREW	28,30,32,34,54	WPP574G	GINGIHUE POST 5MM(D) X 7.5MM(P) X 4MM(H)	27
UNISG	GOLD-TITE SQUARE SCREW	28,30,32,34,54	WPP60	POLISHING PROTECTOR 6MM(D)	59
UNITS	SQUARE TRY-IN SCREW (5PK) 4.1, 5, 6MM(D)	28,30,32,34,54	WPP662G	GINGIHUE POST 6MM(D) X 6MM(P) X 2MM(H)	27
WAB200	STANDARD ABUTMENT 5MM(D) X 2MM(H)	43	WPP664G	GINGIHUE POST 6MM(D) X 6MM(P) X 4MM(H)	27
WAB300	STANDARD ABUTMENT 5MM(D) X 3MM(H)	43	WPP672G	GINGIHUE POST 6MM(D) X 7.5MM(P) X 2MM(H)	27
WAB400	STANDARD ABUTMENT 5MM(D) X 4MM(H)	43	WPP674G	GINGIHUE POST 6MM(D) X 7.5MM(P) X 4MM(H)	27
WAB550	STANDARD ABUTMENT 5MM(D) X 5.5MM(H)	43	WSK10	WAXING SCREW/GUIDE PIN-KNURLED 10MM(L)	16,20,38,42,54
WCAP564	ZIREAL® POST 5MM(D) X 6MM(P) X 4MM(H)	29	WSK15	WAXING SCREW/GUIDE PIN-KNURLED 15MM(L)	16,20,38,42,54
WCAP574	ZIREAL POST 5MM(D) X 7.5MM(P) X 4MM(H)	29	WSK30	WAXING SCREW/GUIDE PIN-KNURLED 20MM(L)	54
WCLA6	CONICAL ABUTMENT LAB ANALOG 6MM(D)	18,40	WSU30	KNURLED IMPLANT WAXING SCREW/GUIDE PIN	54
WCP661	CONICAL EP® PICK-UP COPING (HEXED) 6MM(D) X 6MM(P)	18,40	WTCS51	TEMPORARY (HEXED) IMPLANT CYLINDER 5MM(D)	34
WCP662	CONICAL EP PICK-UP COPING (NON-HEXED) 6MM(D) X 6MM(P)	18,40	WTCS52	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 5MM(D)	34
WCP671	CONICAL EP PICK-UP COPING (HEXED) 6MM(D) X 7.5MM(P)	18,40	WTCS61	TEMPORARY (HEXED) IMPLANT CYLINDER 6MM(D)	34
WCPP6	POLISHING PROTECTOR CONICAL ABUTMENT 6MM	18,40,59	WTCS62	TEMPORARY (NON-HEXED) IMPLANT CYLINDER 6MM(D)	34
WCS66	CONICAL EP HEALING CAP 6MM(D) X 6MM(P)	18,40			
WCS67	CONICAL EP HEALING CAP 6MM(D) X 7.5MM(P)	18,40			
WCT661	CONICAL EP TWIST LOCK COPING (HEXED) 6MM(D) X 6MM(P)	18,40			
WCT662	CONICAL EP TWIST LOCK COPING (NON-HEXED) 6MM(D) X 6MM(P)	18,40			
WCT671	CONICAL EP TWIST LOCK COPING (HEXED) 6MM(D) X 7.5MM(P)	18,40			
WCT672	CONICAL EP TWIST LOCK COPING (NON-HEXED) 6MM(D) X 7.5MM(P)	18,40			
WCTC60	CONICAL TEMPORARY CYLINDER (HEXED) 6MM(D) X 6MM(P)	18,40			
WCTC61	CONICAL TEMPORARY CYLINDER (NON-HEXED) 6MM(D) X 6MM(P)	18,40			
WCTC671	CONICAL TEMPORARY CYLINDER (NON-HEXED) 6MM(D) X 7.5MM(P)	18,40			
WGA51C	UCLA GOLD (HEXED) ABUTMENT CYLINDER 5MM(D)	31,33			

Ordering Information

Some products may not be available outside the U.S.A.
Algunos productos no se comercializan fuera de EE.UU.
Certains produits ne sont pas disponibles en dehors des États-Unis.
Einige Produkte sind außerhalb der USA nicht erhältlich.

To Place an Order:

Contact your local BIOMET **3i**, Inc. Representative or call:
BIOMET **3i**, Inc. Customer Service
Monday–Thursday 8am–8pm (EST)
Friday 8am–6:30pm (EST)
800-342-5454 Fax 561-776-1272
In Canada: 800-363-1980 Outside US: 561-776-6700

TERMS AND CONDITIONS OF SALE. The following are the terms and conditions by which BIOMET **3i**, Inc. sells its products.

GOVERNING TERMS. Any shipment of products shall be deemed to be on the terms and conditions stated herein. Any and all terms and conditions submitted by Purchaser are hereby rejected.

TAXES. The prices set forth herein do not include any sales, use, excise, ad valorem, property or other taxes applicable to the sale, use or delivery of the products, all of which shall be paid by Purchaser separately or added to the contract price and paid by Purchaser to BIOMET **3i**, Inc.

PRICES. The prices set forth for the products are in United States Dollars.

DELIVERY. Products sold hereunder shall be delivered F.O.B. manufacturer's plant or distributor's plant, as applicable. Purchaser shall assume responsibility for all subsequent delivery or shipping charges.

PAYMENT. Payment terms shall be as set forth under the "Terms" section on front of invoice.

WARRANTY. EXCEPT AS EXPRESSLY SET FORTH IN THE "BIOMET **3i**, INC. FIVE YEAR WARRANTY PROGRAM," NEITHER BIOMET **3i**, INC. NOR ANY OF ITS AFFILIATES MAKE ANY WARRANTY, EXPRESS OR IMPLIED, EXCEPT THAT ITS PRODUCTS SHALL BE FREE FROM DEFECTS IN MATERIAL AND/OR WORKMANSHIP. THIS WARRANTY APPLIES ONLY TO THE ORIGINAL PURCHASER. IN THE EVENT OF A PRODUCT DEFECT, IMMEDIATELY NOTIFY BIOMET **3i**, INC. OF THE DEFECT PRIOR TO RETURNING THE PRODUCT. DEVICES SHALL BE STERILIZED PRIOR TO RETURN. AS ITS SOLE OBLIGATION AND AS PURCHASER'S SOLE REMEDY UNDER THIS WARRANTY, BIOMET **3i**, INC. WILL, AT ITS OPTION, EITHER REPAIR, REPLACE OR ISSUE CREDIT FOR SUCH PRODUCTS. PURCHASER ASSUMES ALL RISKS AND LIABILITY RESULTING FROM THE USE OF THESE PRODUCTS, WHETHER USED SEPARATELY OR IN COMBINATION WITH OTHER PRODUCTS.

EXCEPT FOR THE WARRANTY EXPRESSLY DESCRIBED IN "WARRANTY" PARAGRAPH ABOVE, NEITHER BIOMET **3i**, INC. NOR ANY OF ITS AFFILIATES MAKES ANY OTHER WARRANTY WITH RESPECT TO THE BIOMET **3i**, INC. PRODUCTS, EXPRESSED OR IMPLIED, WRITTEN OR ORAL, INCLUDING, WITHOUT LIMITATION, ANY IMPLIED WARRANTY OF MERCHANTABILITY, OR A WARRANTY OF FITNESS FOR A PARTICULAR PURPOSE.

EDUCATION; MODIFICATION OF PRODUCTS. BIOMET **3i**, Inc. strongly recommends completion of formal post graduate implant education and strict adherence to the procedures described in BIOMET **3i**, Inc.'s Implant Instruction Manuals. BIOMET **3i**, Inc. continually strives to improve its products and therefore reserves the right to improve, modify or discontinue products at any time, or to change specifications of the products without notice and without incurring any obligation.

RETURN POLICY. A Purchaser may return any BIOMET **3i**, Inc. Product within 90 days of the invoice date. BIOMET **3i**, Inc. Products returned within 60 days of the invoice date will be accepted without any re-stocking fee to the Purchaser. BIOMET **3i**, Inc. Products returned between 61 and 90 days of the invoice date will be subject to a 15% restocking fee. A BIOMET **3i**, Inc. Product will be accepted for return only if the BIOMET **3i**, Inc. Product is (1) returned in its original, unopened package (including autoclavable products); (2) received by BIOMET **3i**, Inc. within 90 days after the invoice date for that product; and (3) returned freight prepaid to 4555 Riverside Drive, Palm Beach Gardens, Florida 33410, (Attention: Returns Department) accompanied by the BIOMET **3i**, Inc. Return authorization number provided by BIOMET **3i**, Inc.'s Customer Service Department. Purchaser should be advised that BIOMET **3i**, Inc. Products not meeting the above criteria will not be accepted for return.

EXCHANGE POLICY. BIOMET **3i**, Inc. Products may be exchanged within 180 days of the invoice date, without a re-stocking fee, for other BIOMET **3i**, Inc. Products of equal or lesser value within the same product family as determined by

BIOMET **3i**, Inc. (ex. implant for implant, abutment for abutment, membrane for membrane). BIOMET **3i**, Inc. Products may be exchanged within 180 days of the invoice date for other BIOMET **3i**, Inc. Products of greater value within the same product family as determined by BIOMET **3i**, Inc. (ex. implant for implant, abutment for abutment, membrane for membrane), with the price differential paid by the Purchaser. In both cases, the exchanged BIOMET **3i**, Inc. Product must be (1) returned in its original, unopened package (including autoclavable products); (2) a currently offered BIOMET **3i**, Inc. Product (discontinued product not included); and (3) returned freight prepaid to 4555 Riverside Drive, Palm Beach Gardens, Florida 33410, (Attention: Returns Department) and accompanied by the BIOMET **3i**, Inc. Return Authorization Number provided by BIOMET **3i**, Inc.'s Customer Service Department.

LICENSES, PERMITS AND EXPORT CONTROL. The timely securing of permits, licenses or other local, state or federal governmental approvals required in connection with Purchaser's use of any products hereunder shall be the sole responsibility of Purchaser and Purchaser shall bear the cost thereof. Unless otherwise agreed between BIOMET **3i**, Inc. and Purchaser, products sold hereunder are only for use in the United States. Purchaser agrees that the Purchaser will comply fully with all applicable state and federal laws and regulations and Purchaser shall indemnify BIOMET **3i**, Inc. for all losses, damages and penalties incurred as a result of any violation of applicable state or federal law or regulations.

The advertised devices may not have been licensed in accordance with Canadian Law.

FORCE MAJEURE. BIOMET **3i**, Inc. shall not be liable for any loss or damage due to failure or delay arising out of any cause beyond the reasonable control of BIOMET **3i**, Inc. In the event of any failure or delay resulting from such causes, an equitable adjustment of delivery and any other appropriate terms and conditions shall be made. No such failure or delay shall be the basis for an increase in BIOMET **3i**, Inc.'s obligations nor any termination by Purchaser.

LIMITATION OF LIABILITY. UNDER NO CIRCUMSTANCES SHALL BIOMET **3i**, INC. OR ANY OF ITS AFFILIATES BE LIABLE FOR BUSINESS INTERRUPTION, LOSS OF PROFITS, SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES OF ANY NATURE AND FROM ANY CAUSE WHETHER BASED IN CONTRACT, WARRANTY OR TORT (INCLUDING NEGLIGENCE) OR OTHER LEGAL THEORY, EVEN IF BIOMET **3i**, INC. HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

VALIDITY. If any provision of these Terms and Conditions is found to be illegal or unenforceable in any respect, such illegality or unenforceability shall not affect any other provision of these Terms and Conditions, all of which shall remain enforceable in accordance with their terms.

GENERAL PROVISIONS. The purchase of the products and these Terms and Conditions are governed by the laws of Florida, without regard to conflicts of law principles. This document incorporates all oral and written representations between the parties and constitutes the entire agreement and understanding of the parties with respect to the subject matter hereof and supercedes any and all other agreements either oral or written between the parties with respect to such subject matter. No amendment or modification may be made to this document unless in writing and duly executed by an authorized representative of BIOMET **3i**, Inc.

CAUTION. Federal (U.S.) Law restricts these devices to sale by or on the order of a licensed healthcare practitioner. Devices labeled "STERILE" are certified to be sterile unless sterile package is opened or damaged.

EXPORT ORDERS. Require advance payment or letter of credit. Shipments are made either freight collect or paid by BIOMET **3i**, Inc. and added to invoice. Unless special instructions are received with the order, the shipping method will be determined by BIOMET **3i**, Inc., F.O.B. Palm Beach Gardens, FL.

TRADEMARKS. BIOMET **3i** LLC. Registered Trademarks®: BIOMET **3i** and design, ACT, Advanced Cutting Technology, ARCHITECH PSR, Biogran, CAM StructSURE, Certain, DIEM, Encode, EP, GingiHue, Gold-Tite, IOL, Miniplant, Navigator, OSSEOCISION, OsseoGuard, OSSEOTITE, OSSEOTITE XP, PreFormance, Prep-Tite, PREVAIL, Provide, QuickBridge, QuickSeat, RegenerOss and ZiReal are registered trademarks of BIOMET **3i** LLC.

BIOMET **3i** LLC. Trademarks™: BIOMET **3i**, BIOMET **3i** IDS, Gold Standard ZR, ICE, NanoTite, Providing Solutions – One Patient At A Time and Twist Lock are trademarks of BIOMET **3i** LLC.

Biomet is a registered trademark of BIOMET, Inc. Calcigen is a trademark of BIOMET, Inc. Dolder is a registered trademark of Prof. Eugen Dolder, formerly the director of the School of Dentistry at the University of Zurich. Endobon is a registered trademark of BIOMET Deutschland GmbH. LOCATOR is a registered trademark of Zest Anchors, Inc. Safescraper is a registered trademark of CGM S.p.A. Divisione Medica META.

SUBSIDIARIES

AUSTRALIA

Phone: +61-2-9855-4444
Fax: +61-2-9888-9900

AUSTRIA

Phone: +43-(0)8000-700-17
Fax: +43-(0)8000-700-18

BELGIUM

Phone: +32-2-5410290
Fax: +32-2-5410291

BRAZIL

Phone: +55-11-5081-4405
Fax: +55-11-5081-7484

CANADA

Phone: +514-956-9843
Fax: +514-956-9844

FRANCE

Phone: +33-1-41054343
Fax: +33-1-41054340

GERMANY

Phone: +49-(0)800-101-64-20
Fax: +49-(0)800-313-11-11

IRELAND

Phone: +353-1-800-552-752
Fax: +44-1628-820182

JAPAN

Phone: +81-66868-3012
Fax: +81-66868-2444

KOREA

Phone: +82-2-5678-550
Fax: +82-2-5678-577

MEXICO

Phone: +52-55-2282-0120
Fax: +52-55-2282-0120 ext. 20

THE NETHERLANDS

Phone: +31-(0)78-629-2800
Fax: +31-(0)78-629-2801

NEW ZEALAND

Phone: +64-508-122-221
Fax: +64-508-133-331

NORDIC REGION

Phone: +46-40-17-6090
Fax: +46-40-17-6099

PORTUGAL

Phone: +34-902-34-34-31
Fax: +34-93-445-81-36
+351-21-000-16-75

SPAIN

Phone: +34-902-34-34-31
Fax: +34-93-445-81-36

SWITZERLAND

Phone: +41-(0)800-24-66-38
Fax: +41-(0)800-24-66-39

U.K.

Phone: +44-800-652-1233
Fax: +44-1628-820182

DISTRIBUTORS

ARGENTINA

Dentalmax, SA
Phone: +541-1482-71001
Fax: +541-1482-67373

CHILE

Cybel, SA
Phone: +56-2-2321883
Fax: +56-2-2330176

CHINA

Atek Inc.
Phone: +86-21-6329-1265
Fax: +86-21-6329-1620

COLOMBIA

3i Colombia
Phone: +571-612-9362
Fax: +571-620-6412

COSTA RICA

Implantec S.A.
Phone: +506-234-9043
Fax: +506-224-7620

EL SALVADOR

Dentimere SA de CV
Phone: +503-263-6350
Fax: +503-263-6676

GREECE

Impladend Dental Implants, LLC
Phone: +30-2310-501-651
Fax: +30-2310-862-090

ISRAEL

H.A. Systems
Phone: +972-3-6138777
Fax: +972-3-6138778

HONG KONG

Ositek Inc., Ltd.
Phone: +852-8121-6601
Fax: +852-3747-3754

ITALY

Biomax spa
Phone: +39-0444-913410
Fax: +39-0444-913695

MIDDLE EAST

3i MENA s.a.l.
Middle East And North Africa
Phone: +961-1-694000
Fax: +961-1-694222

PARAGUAY

Andres H. Arce y Cia SRL
Phone: +595-21-208185
Fax: +595-21-496291

POLAND

Dental Depot Wasio
Phone: +48 71 335 70 71
Fax: +48 71 335 70 90

RUSSIA

Com-Dental
Phone: +7-495-580-3080
Fax: +7-495-580-3081

SINGAPORE

Asia Implant Support & Services
Phone: +65-6223-2229
Fax: +65-6220-3538

SOUTH AFRICA

Selective Aesthetics
Phone: +27-11-991-7068
Fax: +27-11-672-1391

TAIWAN

Kuo Hwa Dental Suppliers Co., Ltd.
Phone: +886-2-2226-1770
Fax: +886-2-2226-8747

THAILAND

3i (Thailand) Co., LTD.
Phone: +662-252-6685
Fax: +662-252-6686

TURKEY

Tamer Med. A.Ş.-Turkey
Phone: +90-212-465-3352
Fax: +90-212-465-3502

UKRAINE

Victoria Premium
Phone: +38-044-331-10-09
Fax: +38-044-331-10-70

URUGUAY

ProSimplant S.R.L.
Phone: +598-2-4034163
Fax: +598-2-4034163

VIETNAM

D.O.E.
(Dentistry Of Excellence Vietnam)
Phone: +84 89 25 37 03
Fax: +84 89 25 37 00



CATRES
REV B 02/11

**To Receive Information About 's Products, Services And Events By Email,
Please Visit Our Website At www.biomet3i.com**

Not Available In All Markets, Please Consult Your Local  Sales Representative For Availability